

IAEA Analytical Quality in Nuclear Applications Series No. 36

# Worldwide Open Proficiency Test for X Ray Fluorescence Laboratories PTXRFIAEA09: Determination of Major, Minor and Trace Elements in a River Clay



**WORLDWIDE OPEN PROFICIENCY  
TEST FOR X RAY FLUORESCENCE  
LABORATORIES PTXRFIAEA09:  
DETERMINATION OF MAJOR, MINOR  
AND TRACE ELEMENTS IN A RIVER CLAY**

The following States are Members of the International Atomic Energy Agency:

AFGHANISTAN	GHANA	OMAN
ALBANIA	GREECE	PAKISTAN
ALGERIA	GUATEMALA	PALAU
ANGOLA	HAITI	PANAMA
ARGENTINA	HOLY SEE	PAPUA NEW GUINEA
ARMENIA	HONDURAS	PARAGUAY
AUSTRALIA	HUNGARY	PERU
AUSTRIA	ICELAND	PHILIPPINES
AZERBAIJAN	INDIA	POLAND
BAHAMAS	INDONESIA	PORTUGAL
BAHRAIN	IRAN, ISLAMIC REPUBLIC OF	QATAR
BANGLADESH	IRAQ	REPUBLIC OF MOLDOVA
BELARUS	IRELAND	ROMANIA
BELGIUM	ISRAEL	RUSSIAN FEDERATION
BELIZE	ITALY	RWANDA
BENIN	JAMAICA	SAN MARINO
BOLIVIA	JAPAN	SAUDI ARABIA
BOSNIA AND HERZEGOVINA	JORDAN	SENEGAL
BOTSWANA	KAZAKHSTAN	SERBIA
BRAZIL	KENYA	SEYCHELLES
BRUNEI DARUSSALAM	KOREA, REPUBLIC OF	SIERRA LEONE
BULGARIA	KUWAIT	SINGAPORE
BURKINA FASO	KYRGYZSTAN	SLOVAKIA
BURUNDI	LAO PEOPLE'S DEMOCRATIC REPUBLIC	SLOVENIA
CAMBODIA	LATVIA	SOUTH AFRICA
CAMEROON	LEBANON	SPAIN
CANADA	LESOTHO	SRI LANKA
CENTRAL AFRICAN REPUBLIC	LIBERIA	SUDAN
CHAD	LIBYA	SWAZILAND
CHILE	LIECHTENSTEIN	SWEDEN
CHINA	LITHUANIA	SWITZERLAND
COLOMBIA	LUXEMBOURG	SYRIAN ARAB REPUBLIC
CONGO	MADAGASCAR	TAJIKISTAN
COSTA RICA	MALAWI	THAILAND
CÔTE D'IVOIRE	MALAYSIA	THE FORMER YUGOSLAV REPUBLIC OF MACEDONIA
CROATIA	MALI	TOGO
CUBA	MALTA	TRINIDAD AND TOBAGO
CYPRUS	MARSHALL ISLANDS	TUNISIA
CZECH REPUBLIC	MAURITANIA, ISLAMIC REPUBLIC OF	TURKEY
DEMOCRATIC REPUBLIC OF THE CONGO	MAURITIUS	UGANDA
DENMARK	MEXICO	UKRAINE
DOMINICA	MONACO	UNITED ARAB EMIRATES
DOMINICAN REPUBLIC	MONGOLIA	UNITED KINGDOM OF GREAT BRITAIN AND NORTHERN IRELAND
ECUADOR	MONTENEGRO	UNITED REPUBLIC OF TANZANIA
EGYPT	MOROCCO	UNITED STATES OF AMERICA
EL SALVADOR	MOZAMBIQUE	URUGUAY
ERITREA	MYANMAR	UZBEKISTAN
ESTONIA	NAMIBIA	VENEZUELA, BOLIVARIAN REPUBLIC OF
ETHIOPIA	NEPAL	VIET NAM
FIJI	NETHERLANDS	YEMEN
FINLAND	NEW ZEALAND	ZAMBIA
FRANCE	NICARAGUA	ZIMBABWE
GABON	NIGER	
GEORGIA	NIGERIA	
GERMANY	NORWAY	

The Agency's Statute was approved on 23 October 1956 by the Conference on the Statute of the IAEA held at United Nations Headquarters, New York; it entered into force on 29 July 1957. The Headquarters of the Agency are situated in Vienna. Its principal objective is "to accelerate and enlarge the contribution of atomic energy to peace, health and prosperity throughout the world".

**WORLDWIDE OPEN PROFICIENCY  
TEST FOR X RAY FLUORESCENCE  
LABORATORIES PTXRFIAEA09:  
DETERMINATION OF MAJOR, MINOR  
AND TRACE ELEMENTS IN A RIVER CLAY**

## COPYRIGHT NOTICE

All IAEA scientific and technical publications are protected by the terms of the Universal Copyright Convention as adopted in 1952 (Berne) and as revised in 1972 (Paris). The copyright has since been extended by the World Intellectual Property Organization (Geneva) to include electronic and virtual intellectual property. Permission to use whole or parts of texts contained in IAEA publications in printed or electronic form must be obtained and is usually subject to royalty agreements. Proposals for non-commercial reproductions and translations are welcomed and considered on a case-by-case basis. Enquiries should be addressed to the IAEA Publishing Section at:

Marketing and Sales Unit, Publishing Section  
International Atomic Energy Agency  
Vienna International Centre  
PO Box 100  
1400 Vienna, Austria  
fax: +43 1 2600 29302  
tel.: +43 1 2600 22417  
email: [sales.publications@iaea.org](mailto:sales.publications@iaea.org)  
<http://www.iaea.org/books>

For further information on this publication, please contact:

Physics Section  
International Atomic Energy Agency  
2444 Seibersdorf  
Austria  
Email: [Official.Mail@iaea.org](mailto:Official.Mail@iaea.org)

WORLDWIDE OPEN PROFICIENCY TEST FOR X RAY FLUORESCENCE LABORATORIES PTXRFIAEA09:  
DETERMINATION OF MAJOR, MINOR AND TRACE ELEMENTS IN A RIVER CLAY

IAEA, VIENNA, 2014  
IAEA/AQ/36  
ISSN 2074-7659  
© IAEA, 2014  
Printed by the IAEA in Austria  
October 2014

## **FOREWORD**

The IAEA assists Member State laboratories to maintain their readiness by producing reference materials, developing standardized analytical methods, and conducting interlaboratory comparisons and proficiency tests as tools for quality control. To ensure a reliable, worldwide, rapid and consistent response, the IAEA Nuclear Spectrometry and Applications Laboratory organizes tests for Member State laboratories.

This publication presents the results of the worldwide proficiency test PTXRFIAEA09 on the determination of major, minor and trace elements in river clay. Methodologies, a data evaluation approach, a summary evaluation of each element and individual evaluation reports for each laboratory are also described. The test was carried out within the IAEA project Nuclear Spectrometry for Analytical Applications, under the Nuclear Science Programme. The main objective of the project was to enhance the capability of interested Member States in effective utilization of nuclear spectrometries and analytical services in industry, human health and agriculture, and in monitoring and evaluating environmental pollution.

This proficiency test was designed to identify analytical problems and to support Member State laboratories in improving the quality of their analytical results, maintaining their accreditation and providing a regular forum for discussion and technology transfer in this area. The type of sample and the concentration levels of the analytes were designed to enable the identification of potential analytical problems.

The IAEA officer responsible for this publication was A. Migliori of the Division of Physical and Chemical Sciences.

#### *EDITORIAL NOTE*

*This publication has been prepared from the original material as submitted by the contributors and has not been edited by the editorial staff of the IAEA. The views expressed remain the responsibility of the contributors and do not necessarily reflect those of the IAEA or the governments of its Member States.*

*This publication has not been edited by the editorial staff of the IAEA. It does not address questions of responsibility, legal or otherwise, for acts or omissions on the part of any person.*

*The use of particular designations of countries or territories does not imply any judgement by the publisher, the IAEA, as to the legal status of such countries or territories, of their authorities and institutions or of the delimitation of their boundaries.*

*The mention of names of specific companies or products (whether or not indicated as registered) does not imply any intention to infringe proprietary rights, nor should it be construed as an endorsement or recommendation on the part of the IAEA.*

*The contributors are responsible for having obtained the necessary permission for the IAEA to reproduce, translate or use material from sources already protected by copyrights.*

*The IAEA has no responsibility for the persistence or accuracy of URLs for external or third party Internet web sites referred to in this publication and does not guarantee that any content on such web sites is, or will remain, accurate or appropriate.*

## CONTENTS

1.	INTRODUCTION.....	1
2.	DESCRIPTION OF THE TEST SAMPLE .....	1
3.	DETAILS OF THE EXERCISE .....	1
3.1.	ASSIGNED VALUE AND TARGET STANDARD DEVIATION.....	1
3.2.	<i>z</i> -SCORES AND <i>u</i> -SCORES.....	2
3.3.	CONSENSUS VALUES .....	4
4.	RESULTS .....	7
	REFERENCES.....	83
	GLOSSARY.....	85
	LIST OF CONTRIBUTORS TO DRAFTING AND REVIEW.....	87



## **1. INTRODUCTION**

The PTXRFIAEA09 proficiency test aimed at analytical laboratories applying X-ray fluorescence (XRF) techniques in environmental monitoring. The participants were requested to use their established and proven analytical procedures for the determination of concentrations of chemical elements in a river clay sample.

River clay test samples with established homogeneity and well characterized known target values of the mass fractions of analytes were distributed to participating laboratories. The laboratories were requested to analyse the sample using established techniques following their analytical procedures. Based on the results of the proficiency test presented in the report, each participating laboratory should assess its analytical performance by using the specified criteria and, if appropriate, to identify discrepancies, and to correct relevant analytical procedures.

The samples, together with detailed instructions for analysts, were distributed to the participating laboratories in May 2012. The deadline for submission of the results was September 15, 2012. The last results were received in October 31, 2012. The submitted results were processed, grouped versus analytes/laboratories and compared with the analytes' assigned values. The values of  $z$ - and of  $u$ -scores were calculated for three fit-for-purpose levels. For the definitions of the  $z$ - and  $u$ -scores please see Section 3.2. The obtained results as well as the description of the data evaluation procedures have been presented in this report. Each laboratory was assigned a code, therefore full anonymity of the presented results is guaranteed. The link between the laboratory code and the laboratory name is known only to the organisers of the proficiency test and to the laboratory itself.

## **2. DESCRIPTION OF THE TEST SAMPLE**

The test sample was a river clay material prepared and tested by an external independent laboratory. The powdered, homogenized and dried material was distributed to 42 laboratories in sealed plastic bottles, each bottle containing 100 g of the test sample. The participants were asked to conduct the determination of the mass fractions of chemical elements making up the sample according to their routine analytical procedures. They were also instructed to determine the moisture content of the material by using a separate sample and to report the results on a dry-weight basis. Only one result per element per analytical technique should be submitted. Each result should be accompanied by an estimate of its uncertainty expressed as one standard deviation. No restriction on the number of the reported elements was imposed.

## **3. DETAILS OF THE EXERCISE**

### **3.1. ASSIGNED VALUE AND TARGET STANDARD DEVIATION**

The reference values supplied by the provider of the material, established by independent inter-laboratory survey, were used as the assigned values of the analytes,  $X_A$ . The results for 58 analytes were submitted by participants of this proficiency test: Al, As, Ba, Bi, Br, Ca, Cd, Ce, Cl, Co, Cr, Cs, Cu, Dy, Er, Eu, Fe, Ga, Ge, Hf, Hg, Ho, I, K, La, Lu, Mg, Mn, Mo, Na, Nb, Nd, Ni, P, Pb, Pr, Rb, S, Sb, Sc, Se, Si, Sm, Sn, Sr, Ta, Tb, Th, Ti, Tl, Tm, U, V, W, Y, Yb, Zn and Zr.

The  $z$ - and  $u$ -scores were calculated for all the submitted results of all analytes except Bi, Cl, Cs, Dy, Er, Eu, Ge, Hf, Ho, I, Lu, Mo, Pr, Se, Sm, Ta, Tb, Tm, W and Yb, for which the assigned values were not available.

For each analyte a target value of the standard deviation has been assigned using a modified Horowitz function as proposed in the reference [1]:

$$H_A = \begin{cases} 0.22X_A & X_A < 1.2 \cdot 10^{-7} \\ 0.02(X_A)^{0.8495} & 1.2 \cdot 10^{-7} \leq X_A \leq 0.138 \\ 0.01\sqrt{X_A} & X_A > 0.138 \end{cases} \quad (1)$$

In Eqn. (1) the assigned value of analyte,  $X_A$ , is expressed as a mass fraction. The target value of the standard deviation,  $\sigma_A$  is related to  $H_A$  by a factor  $k$ :

$$\sigma_A = kH_A, \quad k = 0.5, 1.0, 1.5 \quad (2)$$

Depending on the value of the factor  $k$  the target value of the standard deviation is recognized as fit-for-purpose at three levels of uncertainty:  $k = 0.5$  - appropriate for high precision analysis;  $k = 1.0$  - appropriate for well-established routine analysis;  $k = 1.5$  - satisfactory for common analytical tasks. The relative value of the target standard deviation,  $RSD$ , expressed in per cent, is defined as follows:

$$RSD = \frac{\sigma_A}{X_A} \cdot 100\% \quad (3)$$

The relative value of the target standard deviation as a function of the assigned mass fraction of the analyte,  $X_A$ , is shown in Fig. 1 for the three different values of the  $k$  factor.

### 3.2. $z$ -SCORES AND $u$ -SCORES

The reported concentrations of analytes were compared with the assigned values by using the  $z$ -score analysis. For every result a  $z$ -score was calculated:

$$z = \frac{x - X_A}{\sigma_A} \quad (4)$$

The term ‘ $x$ ’ denotes the reported mass fraction of analyte. Defined by different fit-for-purpose ranges of the target standard deviation, three different values of  $z$ -scores were calculated by combining Eqns. (2) and (4). Assuming that appropriate values for  $X_A$  and  $\sigma_A$  have been used and that the underlying distribution of analytical errors is normal, apart from outliers, in a well-behaved analytical system  $z$ -scores would be expected to fall outside the range  $-2 \leq z \leq 2$  in about 4.6% of instances, and outside the range  $-3 < z < 3$  only in about 0.3%. Therefore, based on the  $z$ -scores the following decision limits were established:

$$\begin{aligned} |z| \leq 2 & \quad - \text{a satisfactory result} \\ 2 < |z| < 3 & \quad - \text{the result is considered questionable} \\ |z| \geq 3 & \quad - \text{the result is considered unsatisfactory} \end{aligned} \quad (5)$$

The advice to the laboratory is that, independent of the fit-for-purpose range selected by the laboratory, any  $z$ -score for an element outside the range  $-2 \leq z \leq 2$  should be examined by the

analyst and all steps of the analytical procedure verified to identify the source(s) of the analytical bias.

For every participant the rescaled sum of  $z$ -scores,  $RSZ$ , as well as the sum of squared  $z$ -scores,  $SSZ$ , were calculated as defined by the following equations:

$$RSZ = \frac{\sum_{i=1}^L z_i}{\sqrt{L}} \quad (6)$$

$$SSZ = \sum_{i=1}^L (z_i)^2 \quad (7)$$

The symbol ‘ $L$ ’ denotes the number of results provided by the laboratory/participant for all the analytes determined. The summing up in Eqns. (6) and (7) takes into account all  $z$ -scores for all analytes with known assigned values reported by participant. The  $RSZ$  can be interpreted as a standardized normally distributed variable, with expected value equal to zero and unit variance. It is sensitive in detecting a small consistent bias in an analytical system, however, it is not sensitive in cases where there are even big errors but having opposite signs. The  $SSZ$  takes no account of the signs because it depends on the squared  $z$ -scores. It has a chi-squared ( $\chi^2$ ) distribution with  $L$  degrees of freedom. The  $SSZ$  can be regarded as complementary to  $RSZ$ , which means that if  $RSZ$  is well within the range  $-3 < RSZ < 3$  and if at the same time the value of  $SSZ$  is above the  $\chi^2_{critical}$  value the overall performance of the laboratory requires improvement.

The reported results were accompanied by the standard uncertainty estimate made by the participant. The values were used to calculate  $u$ -scores:

$$u = \frac{|x - X_A|}{\sqrt{(\sigma_A)^2 + (\sigma_x)^2}} \quad (8)$$

The symbol ‘ $\sigma_x$ ’ denotes the standard uncertainty of the submitted result  $x$ . If the assumptions about  $X_A$  and  $\sigma_A$  and about the normality of the underlying distributions are correct, and the laboratory estimate of  $\sigma_x$  takes into account all the significant sources of uncertainty, the  $u$ -scores would have a truncated normal distribution with unit variance. In a well-behaved analytical system only 0.1% of  $u$ -scores would fall outside the range  $u < 3.29$ . Therefore, the following decision limits for the  $u$ -scores were established:

- |                      |  |
|----------------------|--|
| $u \leq 1.64$        | - reported result does not differ from the assigned value          |
| $1.64 < u \leq 1.95$ | - reported result probably does not differ from the assigned value |
| $1.95 < u \leq 2.58$ | - it is not clear whether the reported and assigned values differ  |
| $2.58 < u \leq 3.29$ | - reported result is probably different from the assigned value    |
| $3.29 < u$           | - reported result differs from the assigned value                  |
- (9)

The  $u$ -scores are especially useful for deciding whether the laboratory fit-for-purpose criteria are fulfilled. By comparing Eqn. (4) and Eqn. (8) one can notice that for corresponding values of  $u$ -score and  $z$ -score the following inequality is always fulfilled:

$$u \leq |z| \quad (10)$$

It implies that if the  $u$ -score is larger than 3.29 also the decision limit for the corresponding  $z$ -score is triggered and the laboratory has to check the analytical procedure as well as review the uncertainty budget estimation. If  $u$ -score stays below the value of 1.64 and at the same time the  $z$ -score decision limit is triggered ( $|z| > 3$ ) the laboratory should reevaluate its fit-for-purpose status for that particular analyte.

### 3.3. CONSENSUS VALUES

To examine the overall performance of the participating laboratories the submitted results have been statistically processed and the consensus values were calculated. The results were tested for the presence of outliers using a set of seven outlier rejection tests, shown below:

Description of symbols:

$$\begin{aligned} x_1 < \dots < x_n & \quad - \text{set of analytical results} \\ \bar{x} & \quad - \text{mean value} \\ s & \quad - \text{standard deviation} \end{aligned} \tag{11}$$

- Coefficient of kurtosis [2], number of results:  $5 \leq n \leq 100$ , two-sided test, confidence level = 0.95:

$$b_2 = \frac{n \sum_{i=1}^n (\bar{x} - x_i)^4}{\left[ \sum_{i=1}^n (\bar{x} - x_i)^2 \right]^2} \tag{12}$$

If  $b_2 >$  critical value then reject the result that is at the furthest distance from the mean, decrease  $n$ , repeat the procedure until  $b_2 \leq$  critical value.

- Coefficient of skewness [2], number of results,  $5 \leq n \leq 60$ , one-sided test, confidence level = 0.95:

$$\sqrt{b_1} = \frac{\sqrt{n} \sum_{i=1}^n (x_i - \bar{x})^3}{\left[ \sum_{i=1}^n (x_i - \bar{x})^2 \right]^{3/2}} \tag{13}$$

If  $|\sqrt{b_1}| >$  critical value then: if  $\sqrt{b_1}$  is positive then reject  $x_n$ , otherwise reject  $x_1$ , decrease  $n$ , repeat the procedure until  $|\sqrt{b_1}| \leq$  critical value.

- Veglia's test [3,4], number of results:  $4 \leq n \leq \infty$ , two-sided test, confidence level = 0.95:

$$h = \sqrt{\frac{n}{n-1}} \frac{|x_k - \bar{x}_{n-1}|}{s_{n-1}} \quad (14)$$

where:

$x_k$ , examined value, the result at the furthest distance from the mean;

$\bar{x}_{n-1}$ , the mean value of the population of the results with the examined result excluded;

$s_{n-1}$ , the standard deviation of the population of the results with the examined result excluded.

If  $h >$  critical value then reject  $x_k$  otherwise temporarily exclude the  $x_k$  from the population of results and proceed with testing the next outlier candidate, if the following value of  $h >$  critical value then reject both results, decrease  $n$  respectively, repeat the procedure until  $h \leq$  critical value.

4. Dixon's test [5], number of results:  $3 \leq n \leq 25$ , two-sided test, confidence level = 0.95:

If  $x_1$  is at the furthest distance from the mean value, then calculate:

$$r = \begin{cases} (x_2 - x_1) / (x_n - x_1), & 3 \leq n \leq 7 \\ (x_2 - x_1) / (x_{n-1} - x_1), & 8 \leq n \leq 10 \\ (x_3 - x_1) / (x_{n-1} - x_1), & 11 \leq n \leq 13 \\ (x_3 - x_1) / (x_{n-2} - x_1), & 14 \leq n \leq 25 \end{cases} \quad (15a)$$

If  $x_n$  is at the furthest distance from the mean value then calculate:

$$r = \begin{cases} (x_n - x_{n-1}) / (x_n - x_1), & 3 \leq n \leq 7 \\ (x_n - x_{n-1}) / (x_n - x_2), & 8 \leq n \leq 10 \\ (x_n - x_{n-2}) / (x_n - x_2), & 11 \leq n \leq 13 \\ (x_n - x_{n-2}) / (x_n - x_3), & 14 \leq n \leq 25 \end{cases} \quad (15b)$$

If  $r >$  critical value then reject the tested result, decrease  $n$ , repeat the procedure until  $r \leq$  critical value.

5. Outlier rejection test proposed in [2], number of results:  $4 \leq n \leq 100$ , two-sided test, confidence level = 0.95:

$$w/s = (x_n - x_1) / s \quad (16)$$

If  $w/s >$  critical value then: if  $x_n - \bar{x} = \bar{x} - x_1$ , reject both  $x_1$  and  $x_n$ , otherwise reject  $x_k$  ( $x_k = x_1$  or  $x_k = x_n$ ), the result that is at the furthest distance from the mean, for the remaining population of results ( $n' = n - 1$ ) calculate:  $T_k = |\bar{x}' - x_k| / s'$ , where:  $\bar{x}'$  is the mean value and  $s'$  is the standard deviation of the population of the results excluding the rejected value  $x_k$ , if  $T_k >$  critical value then reject also the second extreme result, decrease  $n$  respectively, repeat the procedure until  $w/s \leq$  critical value.

6. Outlier rejection test proposed in [6], number of results:  $3 \leq n < \infty$ , two-sided test, confidence level = 0.95:

$$B_4 = |x_k - \bar{x}| / s \quad (17)$$

where:

$x_k$ , examined value

If  $B_4 >$  critical value then reject the tested result, repeat the procedure until  $B_4 \leq$  critical value.

7. Outlier rejection test proposed in [7], number of results:  $3 \leq n \leq 100$ , two-sided test, confidence level = 0.95:

$$S_k^2 / S = \frac{\sum_{i=1, i \neq k}^n (x_i - \bar{x}')^2}{\sum_{i=1, i \neq k}^n (x_i - \bar{x})^2}, \quad k = 1 \text{ or } k = n \quad (18)$$

where:

$x_k$ , examined value, the result at the furthest distance from the mean

$\bar{x}'$ , the mean value of the population of the results with the examined result  $x_k$  excluded

If  $S_k^2 / S >$  critical value then reject  $x_k$ , decrease  $n$ , repeat the procedure until  $S_k^2 / S \leq$  critical value.

The results which passed the outlier rejection procedures were used to calculate the consensus mean value of analyte,  $X_C$ , and corresponding consensus value of its standard deviation,  $\sigma_C$ :

$$X_C = \frac{\sum_{i=1}^m x_i}{m} \quad (19)$$

and

$$\sigma_C = \sqrt{\frac{\sum_{i=1}^m (x_i - X_C)^2}{m(m-1)}} \quad (20)$$

The term  $m$  denotes the number of reported values for a given analyte excluding the outliers rejected by at least one of the outlier rejections tests. The summing up in Eqn. (19) and (20) takes into account only the results which passed all the outlier rejection tests. The obtained consensus values were compared with the assigned values of analytes.

## 4. RESULTS

The river clay test sample was distributed to 42 laboratories for chemical composition analysis. Out of the 42 laboratories, 33 participated in the test submitting 673 individual results for 58 chemical elements. The list of the participating laboratories is presented at the end of this report.

The techniques used by the participants and their codes are listed in Table 1.

The techniques EDXRFS, EDXRFISOTOP, and EDXRFTUBE should be considered of similar type. The distinction between them (EDXRFISOTOP or EDXRFTUBE) was based on information provided by the participants. In the case that insufficient information was available a generic type technique EDXRF was assumed. All submitted results have been evaluated.

In Table 2 a summary of the assigned analyte values, the target values of standard deviation (obtained by using modified Horowitz function), the consensus values and their standard deviations are shown. For the elements Bi, Cl, Cs, Dy, Er, Eu, Ge, Hf, Ho, I, Lu, Mo, Pr, Se, Sm, Ta, Tb, Tm, W and Yb the assigned and target values were not available. The consensus values (Eqn. 19) and corresponding standard deviations (Eqn. 20) were calculated based on 587 reported analytical results after excluding 86 results classified as outliers. The correlation between the assigned and the consensus values is shown in Fig. 2.

TABLE 1. THE CODING, DESCRIPTION AND THE ABBREVIATED NAMES OF THE ANALYTICAL TECHNIQUES USED BY PARTICIPANTS OF THE PROFICIENCY TEST EXERCISE

Technique Code	Description	Abbreviation
1.0	Energy dispersive X-ray fluorescence	EDXRFS
1.1	EDXRF, radioisotope excitation	EDXRFISOTOP
1.2	EDXRF, X-ray tube excitation	EDXRFTUBE
1.3	EDXRF, excitation using X-ray tube and secondary targets	EDXRFTUBE-ST
1.4	Total reflection X-ray fluorescence	TXRF
2.0	Wavelength dispersive X-ray fluorescence	WDXRF
5.0	Neutron Activation Analysis	NAA

TABLE 2. THE ASSIGNED VALUES OF ANALYTES, THE TARGET VALUES OF THE STANDARD DEVIATIONS AND THE CONSENSUS VALUES

Analyte symbol	Assigned value of the analyte, $X_A$	Target value of standard deviation, $\sigma_A$			Consensus value of the analyte, $X_C$	Consensus value of the standard deviation, $\sigma_C$	Number of results	Number of outliers
		$k = 0.5$	$k = 1.0$	$k = 1.5$				
[g/kg]								
Al	59.4	0.91	1.82	2.73	59.99	2.99	19	3
Ca	13.8	0.26	0.53	0.79	13.80	0.29	30	4
Fe	29.7	0.50	1.01	1.51	29.79	0.95	33	3
K	19.500	0.35	0.71	1.06	19.87	0.32	29	6
Mg	8.870	0.18	0.36	0.54	10.26	0.50	10	0
Mn	1.000	0.03	0.06	0.08	0.94	0.03	30	4
Na	7.070	0.15	0.30	0.45	7.18	1.21	9	0
P	1.100	0.03	0.06	0.09	1.25	0.18	15	2
Si	322	2.84	5.67	8.51	305.58	4.50	17	4
Ti	4.300	0.10	0.20	0.29	4.38	0.16	30	3
[mg/kg]								
As	13.4	0.73	1.45	2.18	13.70	0.92	16	2
Ba	410	13.26	26.52	39.78	427.12	7.20	14	2
Bi	-	-	-	-	14.84	1.70	1	0
Br	8.39	0.49	0.97	1.46	8.22	0.55	14	1
Cd	0.503	0.04	0.09	0.13	0.51	0.06	3	1
Ce	73.3	3.07	6.14	9.22	78.21	3.34	10	0
Cl	-	-	-	-	690.42	365.93	3	0
Co	12.5	0.68	1.37	2.05	10.66	0.77	11	3
Cr	89.6	3.64	7.29	10.93	91.95	6.98	22	2
Cs	-	-	-	-	8.40	0.31	4	1
Cu	20.1	1.02	2.05	3.07	21.91	1.68	26	5
Dy	-	-	-	-	5.68	1.56	2	0
Er	-	-	-	-	2.92	0.29	1	0
Eu	-	-	-	-	1.34	0.08	2	0
Ga	13.6	0.73	1.47	2.20	12.80	0.78	17	1
Ge	-	-	-	-	2.73	1.05	2	0
Hf	-	-	-	-	7.30	0.59	4	0
Hg	0.05	0.01	0.01	0.02	3.19	1.58	1	0
Ho	-	-	-	-	1.00	0.29	1	0
I	-	-	-	-	5.13	1.76	3	0
La	36.1	1.68	3.37	5.05	37.60	1.41	13	0

Analyte symbol	Assigned value of the analyte, $X_A$	Target value of standard deviation, $\sigma_A$			Consensus value of the analyte, $X_C$	Consensus value of the standard deviation, $\sigma_C$	Number of results	Number of outliers
		$k = 0.5$	$k = 1.0$	$k = 1.5$				
[mg/kg]								
Lu	-	-	-	-	0.40	0.11	3	0
Mo	-	-	-	-	1.52	0.65	3	1
Nb	16.0	0.84	1.69	2.53	14.30	0.75	11	2
Nd	32.7	1.55	3.09	4.64	36.71	3.14	5	0
Ni	37.9	1.75	3.51	5.26	35.93	3.06	21	1
Pb	36.9	1.71	3.43	5.14	37.17	3.13	26	1
Pr	-	-	-	-	7.91	0.05	1	0
Rb	107	4.24	8.47	12.71	105.57	5.77	30	4
S	328	10.97	21.94	32.91	631.32	127.41	13	4
Sb	1.07	0.08	0.17	0.25	1.11	0.10	4	1
Sc	10.2	0.58	1.15	1.73	9.82	0.03	5	3
Se	-	-	-	-	3.47	0.73	1	0
Sm	-	-	-	-	6.51	0.72	3	0
Sn	3.68	0.24	0.48	0.73	9.17	3.50	4	0
Sr	106	4.20	8.40	12.61	101.90	3.03	29	6
Ta	-	-	-	-	266.70	157.30	1	0
Tb	-	-	-	-	1.07	0.23	2	0
Th	11.4	0.63	1.26	1.90	10.84	0.49	12	0
Tl	0.699	0.06	0.12	0.18	1.37	0.00	1	0
Tm	-	-	-	-	855.33	1208.95	2	0
U	2.74	0.19	0.38	0.56	3.13	0.11	6	3
V	80.9	3.34	6.68	10.02	86.85	5.35	20	3
W	-	-	-	-	193.97	22.59	2	0
Y	31.8	1.51	3.02	4.53	27.89	2.15	20	2
Yb	-	-	-	-	2.80	0.38	3	0
Zn	96.1	3.87	7.73	11.60	102.48	3.86	31	4
Zr	302	10.23	20.45	30.68	317.91	14.20	22	3

Table 3 lists the values of the  $z$ - and  $u$ -scores for all submitted results. In brackets next to the element symbol the assigned values of element concentration and the target standard deviation for  $k = 1$  are shown. The  $z$ - and  $u$ -scores were calculated for the three different fit-for-purpose ranges, as defined by Eqn. (2). The results rejected by the outliers rejection procedures were marked with “\*” in the “Analyte concentration” column.

Table 4 shows the combined  $z$ -scores for the three different fit-for-purpose ranges, the  $RSZ$  and  $SSZ$  as defined in Eqns. (6) and (7), for the participating laboratories. The analytes without assigned values (Bi, Cl, Cs, Dy, Er, Eu, Ge, Hf, Ho, I, Lu, Mo, Pr, Se, Sm, Ta, Tb, Tm, W and Yb) were not considered.

Figs. 3-33 and 34-64 present the distributions of the proficiency test results. In Figs 3-33 the individual results are marked with filled circles. The dotted lines show the range of the accepted results (these results were used to calculate the consensus values). The outliers are marked with arrows. Also shown are the estimated parameters of the distribution (after outlier rejection): mode, median, and the mean value. For few elements, the result of density distributions could only be used as indicators of the trends observed in the reported data due to the limited number of results (only density distributions of analytes for which at least 5 results passed the outlier rejection tests are shown). All the populations of results, after outlier rejection, have passed a normality test (Kolmogorov-Smirnov). Figs. 34-64 show the bar chart distributions of the  $z$ -scores for the analytes with at least 6 submitted results. The results are sorted in ascending order versus laboratory/technique code. The bar charts show the distance between the reported and the assigned values of the analyte. The submitted results and their uncertainties are marked with filled squares accompanied by uncertainty bars. The horizontal lines show the admissible levels of  $z$ -score,  $|z| < 2$ , for three different ranges defined by factor  $k$  in Eqn. (2):  $k = 0.5$  (solid black lines),  $k = 1.0$  (solid green lines) and  $k = 1.5$  (solid red lines). The decision levels of satisfactory results,  $|z| < 2$ , for different fit-for-purpose targets have also been marked.

For every participating laboratory its overall performance is presented in Figs. 65-97. The plots presented in this figure relate all the  $u$ -scores and  $z$ -scores calculated for a given laboratory. The hollow symbols denote the values calculated for specific fit-for-purpose levels as defined in Eqn. (2) with factor  $k$ , namely:  $k = 0.5$  (black triangles),  $k = 1.0$  (green circles), and  $k = 1.5$  (red squares). The decision limits of unsatisfactory results are marked with black lines ( $|z| > 3$ ,  $u > 3.29$ ). They divide the plot area in four quadrants. Due to inequality (10) all the points accompanied by a laboratory estimate of the uncertainty fall always below the line  $u = |z|$ . The smaller the laboratory estimate of the uncertainty the closer the related point to the  $u = |z|$  line. Points in the immediate proximity of the dashed diagonal line ( $u = |z|$ ) have underestimated uncertainty values. The well performing laboratories would have more points located in the lower-left quadrant of the plot. If there are many points located in the upper-right quadrant it suggests that these results do not fall in the defined fit-for-purpose targets and that the laboratory provided too “narrow” uncertainty estimate.

Fig. 98 shows the partitioning of the results between different analytical techniques. The largest fraction of analyses, about 83%, was carried out with the energy dispersive spectrometry (EDXRF+TXRF), about 10% with wavelength dispersive mode. Most of the determinations were carried out on samples prepared in the form of pellets (~ 69%), about 5% of the results were obtained after converting the sample to a liquid form by acid digestion or dissolution, about 16% of measurements were carried out on fused beads, and about 10% of analyses were performed without any sample preparation.

TABLE 3. SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED  $z$ -AND  $u$ -SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	$z$ -scores			$u$ -scores		
					$k = 0.5$	$k = 1.0$	$k = 1.5$	$k = 0.5$	$k = 1.0$	$k = 1.5$
Al ( $59.4 \pm 1.82$ ) [g/kg]										
63	1.2	38.13	3.71	9.72	-23.42	-11.71	-7.81	5.58	5.15	4.62
72	1.4	45	1.91	4.25	-15.85	-7.92	-5.28	6.79	5.45	4.32
79	1.3	50.08	10.10	20.16	-10.26	-5.13	-3.42	0.92	0.91	0.89
53	2.0	52.33	5.00	9.55	-7.78	-3.89	-2.59	1.39	1.33	1.24
87	1.3	55.35	0.08	0.14	-4.46	-2.23	-1.49	4.44	2.23	1.49
76	1.3	56.02	1.00	1.78	-3.72	-1.86	-1.24	2.51	1.63	1.16
74	2.0	58.46	0.01	0.01	-1.03	-0.52	-0.34	1.03	0.52	0.34
21	2.0	59.22	0.93	1.57	-0.19	-0.10	-0.06	0.13	0.09	0.06
37	1.2	59.38	0.12	0.21	-0.02	-0.01	-0.01	0.02	0.01	0.01
64	1.1	60	5.00	8.33	0.66	0.33	0.22	0.12	0.11	0.11
77	1.0	61.4	8.30	13.52	2.20	1.10	0.73	0.24	0.24	0.23
55	5.0	62.22	0.19	0.30	3.10	1.55	1.03	3.04	1.54	1.03
58	1.0	64.11	0.31	0.48	5.18	2.59	1.73	4.91	2.56	1.72
86	1.2	74.81	0.58	0.77	16.96	8.48	5.65	14.31	8.08	5.53
69	1.1	76	4.29	5.64	18.27	9.14	6.09	3.79	3.56	3.27
85	1.3	87.24	8.80	10.09	30.64	15.32	10.21	3.15	3.10	3.02
73	1.0	163.94*	4.35	2.66	115.06	57.53	38.35	23.50	22.16	20.35
68	1.3	250.78*	1.63	0.65	210.65	105.33	70.22	102.57	78.41	60.27
70	1.2	390.25*	66.10	16.94	364.16	182.08	121.39	5.00	5.00	5.00
Ca ( $13.8 \pm 0.53$ ) [g/kg]										
84	1.2	7.23*	0.58	7.99	-24.97	-12.49	-8.32	10.34	8.40	6.71
71	1.1	10.53	2.15	20.45	-12.43	-6.22	-4.14	1.51	1.47	1.43
62	1.3	11.14	0.26	2.33	-10.12	-5.06	-3.37	7.19	4.53	3.20
72	1.4	11.47	0.15	1.30	-8.88	-4.44	-2.96	7.72	4.27	2.91
4	1.1	11.8	3.37	28.57	-7.61	-3.80	-2.54	0.59	0.59	0.58
78	1.1	12.58	0.002	0.02	-4.61	-2.31	-1.54	4.61	2.31	1.54
79	1.3	12.78	0.23	1.78	-3.88	-1.94	-1.29	2.93	1.78	1.24
37	1.2	13.08	0.05	0.39	-2.75	-1.38	-0.92	2.70	1.37	0.91
63	1.2	13.19	1.45	10.99	-2.30	-1.15	-0.77	0.41	0.39	0.37
15	1.3	13.32	1.05	7.88	-1.83	-0.91	-0.61	0.44	0.41	0.37
69	1.1	13.5	0.72	5.30	-1.14	-0.57	-0.38	0.39	0.34	0.28
53	2.0	13.55	1.30	9.59	-0.95	-0.48	-0.32	0.19	0.18	0.16
77	1.0	13.6	0.36	2.65	-0.76	-0.38	-0.25	0.45	0.31	0.23
74	2.0	13.66	0.0006	0.004	-0.54	-0.27	-0.18	0.54	0.27	0.18
21	2.0	13.7	0.42	3.07	-0.38	-0.19	-0.13	0.20	0.15	0.11
88	1.0	13.97	1.22	8.76	0.63	0.32	0.21	0.13	0.13	0.11
56	1.3	14.17	0.50	3.53	1.40	0.70	0.47	0.65	0.51	0.39
55	5.0	14.53	0.81	5.60	2.79	1.40	0.93	0.86	0.76	0.65
58	1.0	14.76	0.45	3.05	3.65	1.83	1.22	1.84	1.39	1.06
54	1.0	15.03	2.26	15.03	4.69	2.34	1.56	0.54	0.53	0.52

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED *z*- AND *u*-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	<i>z</i> -scores			<i>u</i> -scores			<i>k</i> = 1.5
					<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	
76	1.3	15.04	0.57	3.78	4.73	2.36	1.58	1.98	1.60	1.28	
87	1.3	15.08	0.01	0.09	4.87	2.43	1.62	4.86	2.43	1.62	
59	1.2	15.15	0.73	4.84	5.15	2.57	1.72	1.74	1.50	1.26	
86	1.2	15.31	0.12	0.81	5.76	2.88	1.92	5.21	2.80	1.90	
61	5.0	15.5	3.40	21.94	6.47	3.23	2.16	0.50	0.49	0.49	
85	1.3	16.19	0.68	4.21	9.08	4.54	3.03	3.27	2.77	2.29	
64	1.1	16.2	0.75	4.63	9.13	4.56	3.04	3.02	2.62	2.21	
70	1.2	19.21*	1.55	8.05	20.57	10.28	6.86	3.45	3.31	3.12	
68	1.3	36.82*	0.70	1.89	87.57	43.78	29.19	30.89	26.36	21.87	
73	1.0	56.26*	0.18	0.32	161.49	80.74	53.83	133.41	76.42	52.49	
Fe ( $29.7 \pm 1.01$ ) [g/kg]											
84	1.2	17.82	0.14	0.76	-23.57	-11.78	-7.86	22.75	11.68	7.82	
54	1.0	18	1.28	7.09	-23.20	-11.60	-7.73	8.52	7.19	5.91	
4	1.1	21.4	0.68	3.20	-16.46	-8.23	-5.49	9.77	6.81	5.00	
21	2.0	25.83	0.81	3.14	-7.68	-3.84	-2.56	4.05	2.99	2.25	
88	1.0	26.9	2.24	8.31	-5.55	-2.78	-1.85	1.22	1.14	1.04	
72	1.4	27.13	0.40	1.47	-5.10	-2.55	-1.70	4.00	2.37	1.64	
24	1.1	27.25	2.97	10.89	-4.87	-2.43	-1.62	0.82	0.78	0.74	
69	1.1	27.3	1.54	5.64	-4.76	-2.38	-1.59	1.48	1.30	1.11	
53	2.0	27.4	3.00	10.95	-4.56	-2.28	-1.52	0.76	0.73	0.68	
76	1.3	27.8	0.46	1.67	-3.77	-1.89	-1.26	2.77	1.71	1.20	
55	5.0	28.13	0.37	1.30	-3.11	-1.55	-1.04	2.52	1.46	1.01	
57	1.4	28.5	0.40	1.42	-2.37	-1.19	-0.79	1.85	1.10	0.76	
37	1.2	28.73	0.03	0.09	-1.93	-0.96	-0.64	1.92	0.96	0.64	
74	2.0	28.86	0.0006	0.002	-1.67	-0.83	-0.56	1.67	0.83	0.56	
77	1.0	28.9	0.82	2.84	-1.59	-0.79	-0.53	0.83	0.62	0.46	
15	1.3	29.32	1.90	6.48	-0.75	-0.38	-0.25	0.19	0.18	0.16	
58	1.0	29.67	0.42	1.42	-0.06	-0.03	-0.02	0.05	0.03	0.02	
78	1.1	30.55	0.001	0.003	1.68	0.84	0.56	1.68	0.84	0.56	
64	1.1	30.6	0.75	2.45	1.78	0.89	0.59	1.00	0.72	0.53	
56	1.3	30.8	1.00	3.25	2.18	1.09	0.73	0.98	0.77	0.60	
61	5.0	30.87	0.35	1.13	2.32	1.16	0.77	1.91	1.10	0.75	
87	1.3	33.23	0.03	0.09	7.00	3.50	2.33	6.99	3.50	2.33	
86	1.2	33.77	0.28	0.83	8.07	4.03	2.69	7.04	3.88	2.64	
79	1.3	33.84	0.31	0.93	8.21	4.11	2.74	6.98	3.92	2.68	
70	1.2	34.53	0.71	2.05	9.59	4.79	3.20	5.57	3.92	2.89	
71	1.1	34.71	8.21	23.66	9.94	4.97	3.31	0.61	0.61	0.60	
59	1.2	35.92	0.25	0.68	12.34	6.17	4.11	11.10	6.00	4.06	
63	1.2	36.95	2.36	6.39	14.38	7.19	4.79	3.00	2.82	2.58	
62	1.3	37.93	0.18	0.47	16.32	8.16	5.44	15.37	8.03	5.40	
85	1.3	41.1	2.30	5.60	22.61	11.30	7.54	4.84	4.54	4.14	
68	1.3	81.17*	0.13	0.15	102.07	51.04	34.02	99.07	50.65	33.91	
82	1.2	125.08*	3.13	2.50	189.18	94.59	63.06	30.10	29.02	27.45	

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED z- AND u-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	z-scores			u-scores			$k =$ 1.5
					$k = 0.5$	$k = 1.0$	$k = 1.5$	$k = 0.5$	$k = 1.0$		
73	1.0	144.35*	0.22	0.16	227.39	113.69	75.80	207.69	110.97	74.97	
K ( $19.500 \pm 0.71$ ) [g/kg]											
62	1.3	1.548*	0.11	7.11	-50.57	-25.28	-16.86	48.30	24.99	16.77	
4	1.1	6.53*	2.18	33.34	-36.78	-18.39	-12.26	5.88	5.67	5.36	
78	1.1	9.62*	0.004	0.04	-27.82	-13.91	-9.27	27.82	13.91	9.27	
84	1.2	11.95*	0.25	2.11	-21.42	-10.71	-7.14	17.43	10.09	6.95	
72	1.4	16.46	0.38	2.29	-8.61	-4.31	-2.87	5.88	3.80	2.70	
88	1.0	17.73	1.56	8.80	-5.01	-2.50	-1.67	1.10	1.03	0.94	
54	1.0	17.8	0.46	2.57	-4.82	-2.41	-1.61	2.94	2.02	1.47	
56	1.3	18.35	0.70	3.82	-3.27	-1.64	-1.09	1.47	1.16	0.91	
64	1.1	18.7	0.75	4.01	-2.27	-1.13	-0.76	0.97	0.78	0.62	
79	1.3	18.98	0.45	2.37	-1.47	-0.74	-0.49	0.91	0.62	0.45	
74	2.0	19.02	0.002	0.008	-1.35	-0.68	-0.45	1.35	0.68	0.45	
77	1.0	19.2	0.95	4.95	-0.85	-0.43	-0.28	0.30	0.25	0.21	
21	2.0	19.36	0.61	3.13	-0.40	-0.20	-0.13	0.20	0.15	0.12	
55	5.0	19.47	0.37	1.90	-0.07	-0.04	-0.02	0.05	0.03	0.02	
53	2.0	19.71	2.00	10.15	0.60	0.30	0.20	0.10	0.10	0.09	
86	1.2	19.97	0.34	1.68	1.34	0.67	0.45	0.97	0.61	0.43	
15	1.3	20.13	2.13	10.58	1.79	0.89	0.60	0.29	0.28	0.26	
76	1.3	20.15	0.52	2.60	1.84	0.92	0.61	1.02	0.74	0.55	
85	1.3	20.42	0.22	1.08	2.61	1.30	0.87	2.21	1.25	0.85	
58	1.0	20.47	0.13	0.64	2.75	1.38	0.92	2.58	1.35	0.91	
37	1.2	20.6	0.06	0.31	3.12	1.56	1.04	3.07	1.55	1.04	
69	1.1	20.6	1.09	5.29	3.12	1.56	1.04	0.96	0.85	0.72	
87	1.3	20.65	0.05	0.24	3.26	1.63	1.09	3.23	1.63	1.09	
59	1.2	21.55	0.30	1.37	5.81	2.90	1.94	4.45	2.68	1.86	
70	1.2	22.36	0.69	3.08	8.10	4.05	2.70	3.69	2.90	2.26	
63	1.2	22.58	2.39	10.56	8.72	4.36	2.91	1.28	1.24	1.18	
71	1.1	22.64	8.02	35.41	8.91	4.46	2.97	0.39	0.39	0.39	
68	1.3	56.54*	1.03	1.82	105.02	52.51	35.01	34.11	29.73	25.12	
73	1.0	76.81*	0.25	0.33	162.49	81.25	54.16	132.09	76.49	52.68	
Mg ( $8.870 \pm 0.36$ ) [g/kg]											
53	2.0	8.28	0.80	9.66	-3.27	-1.63	-1.09	0.72	0.67	0.61	
74	2.0	8.61	0.004	0.05	-1.43	-0.72	-0.48	1.43	0.72	0.48	
21	2.0	8.95	0.38	4.28	0.47	0.23	0.16	0.20	0.16	0.13	
58	1.0	9.13	0.25	2.74	1.44	0.72	0.48	0.84	0.59	0.44	
76	1.3	9.58	0.08	0.80	3.91	1.95	1.30	3.60	1.91	1.29	
85	1.3	10.15	2.25	22.17	7.09	3.54	2.36	0.57	0.56	0.55	
37	1.2	11.31	0.09	0.78	13.53	6.77	4.51	12.17	6.58	4.45	
86	1.2	11.71	0.26	2.24	15.72	7.86	5.24	8.90	6.36	4.72	
87	1.3	12.2	0.84	6.86	18.44	9.22	6.15	3.89	3.65	3.34	
55	1.2	12.67	0.35	2.73	21.02	10.51	7.01	9.72	7.59	5.90	

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED *z*- AND *u*-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	<i>z</i> -scores			<i>u</i> -scores			<i>k</i> = 1.5
					<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	
Mn ( $1.000 \pm 0.06$ ) [g/kg]											
82	1.2	0.23*	0.01	2.51	-27.31	-13.65	-9.10	26.76	13.58	9.08	
4	1.1	0.35*	0.08	24.01	-22.91	-11.46	-7.64	7.27	6.37	5.41	
87	1.3	0.50	0.001	0.20	-16.59	-8.29	-5.53	16.58	8.29	5.53	
84	1.2	0.56	0.01	1.29	-15.42	-7.71	-5.14	14.93	7.64	5.12	
54	1.0	0.61	0.05	8.66	-13.72	-6.86	-4.57	6.46	5.01	3.88	
37	1.2	0.77	0.01	1.87	-7.99	-3.99	-2.66	7.11	3.87	2.62	
64	1.1	0.83	0.03	3.01	-6.01	-3.01	-2.00	4.50	2.75	1.92	
15	1.3	0.89	0.07	8.23	-4.03	-2.02	-1.34	1.46	1.24	1.02	
70	1.2	0.89	0.10	10.80	-3.91	-1.96	-1.30	1.11	0.99	0.86	
88	1.0	0.9	0.08	8.74	-3.71	-1.86	-1.24	1.26	1.09	0.91	
69	1.1	0.9	0.05	5.91	-3.64	-1.82	-1.21	1.71	1.33	1.03	
72	1.4	0.92	0.01	1.34	-2.82	-1.41	-0.94	2.58	1.38	0.93	
78	1.1	0.93	0.004	0.43	-2.27	-1.13	-0.76	2.25	1.13	0.75	
57	1.4	0.93	0.01	1.55	-2.32	-1.16	-0.77	2.06	1.12	0.76	
77	1.0	0.96	0.06	6.46	-1.41	-0.71	-0.47	0.59	0.48	0.38	
53	2.0	0.96	0.09	9.36	-1.34	-0.67	-0.45	0.40	0.36	0.31	
74	2.0	0.99	0.0004	0.04	-0.30	-0.15	-0.10	0.30	0.15	0.10	
58	1.0	0.99	0.04	3.82	-0.21	-0.11	-0.07	0.13	0.09	0.06	
79	1.3	1	0.01	1.31	0.15	0.07	0.05	0.13	0.07	0.05	
56	1.3	1.02	0.06	5.39	0.74	0.37	0.25	0.34	0.27	0.21	
55	5.0	1.03	0.01	0.70	1.04	0.52	0.35	1.01	0.52	0.34	
71	1.1	1.03	0.23	21.97	1.20	0.60	0.40	0.15	0.14	0.14	
59	1.2	1.07	0.04	3.35	2.62	1.31	0.87	1.62	1.10	0.80	
63	1.2	1.09	0.11	9.60	3.32	1.66	1.11	0.86	0.79	0.70	
21	2.0	1.12	0.03	2.95	4.14	2.07	1.38	2.69	1.79	1.29	
62	1.3	1.14	0.03	2.24	4.88	2.44	1.63	3.62	2.22	1.56	
85	1.3	1.14	0.07	5.70	4.95	2.48	1.65	1.98	1.62	1.31	
76	1.3	1.19	0.07	5.52	6.72	3.36	2.24	2.66	2.19	1.77	
68	1.3	2.7*	0.07	2.67	59.94	29.97	19.98	21.91	18.51	15.23	
73	1.0	4.64*	0.06	1.24	128.79	64.40	42.93	56.92	45.20	35.56	
Na ( $7.070 \pm 0.30$ ) [g/kg]											
85	1.3	2.09	0.06	2.93	-33.45	-16.73	-11.15	30.95	16.38	11.05	
58	1.0	3.42	0.21	6.14	-24.50	-12.25	-8.17	14.18	10.01	7.39	
74	2.0	5.69	0.002	0.03	-9.18	-4.59	-3.06	9.18	4.59	3.06	
37	1.2	6.46	0.40	6.21	-4.07	-2.03	-1.36	1.41	1.21	1.01	
21	2.0	6.92	0.30	4.31	-1.01	-0.50	-0.34	0.45	0.36	0.28	
55	5.0	6.94	0.01	0.10	-0.89	-0.45	-0.30	0.89	0.45	0.30	
61	5.0	7.72	0.28	3.63	4.36	2.18	1.45	2.05	1.59	1.23	
76	1.3	11.78	0.92	7.80	31.64	15.82	10.55	5.06	4.88	4.61	
87	1.3	13.56	1.40	10.33	43.57	21.78	14.52	4.61	4.53	4.42	

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED z- AND u-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	z-scores			u-scores			$k =$ 1.5
					$k = 0.5$	$k = 1.0$	$k = 1.5$	$k = 0.5$	$k = 1.0$	$k = 1.5$	
P ( $1.100 \pm 0.06$ ) [g/kg]											
77	1.0	0.13	0.02	15.04	-31.53	-15.77	-10.51	26.41	14.99	10.27	
87	1.3	0.49	0.04	8.07	-19.89	-9.95	-6.63	12.19	8.36	6.09	
76	1.3	0.63	0.02	3.00	-15.23	-7.62	-5.08	12.95	7.28	4.97	
37	1.2	0.99	0.004	0.41	-3.83	-1.91	-1.28	3.79	1.91	1.28	
58	1.0	1.02	0.03	3.04	-2.61	-1.30	-0.87	1.83	1.16	0.82	
21	2.0	1.07	0.04	3.84	-1.04	-0.52	-0.35	0.63	0.43	0.32	
53	2.0	1.11	0.10	9.01	0.33	0.16	0.11	0.10	0.09	0.07	
74	2.0	1.13	0.01	0.48	0.98	0.49	0.33	0.96	0.49	0.33	
72	1.4	1.46	0.12	8.23	11.89	5.95	3.96	2.93	2.70	2.41	
85	1.3	1.7	0.13	7.37	19.47	9.73	6.49	4.64	4.29	3.85	
63	1.2	1.99	0.38	19.06	29.15	14.58	9.72	2.35	2.32	2.29	
55	1.2	2.13	0.16	7.54	33.57	16.78	11.19	6.30	5.99	5.56	
69	1.1	2.4	0.22	9.33	42.39	21.20	14.13	5.75	5.60	5.37	
68	1.3	4.19*	0.18	4.40	100.80	50.40	33.60	16.55	15.92	15.01	
73	1.0	7.68*	0.42	5.49	214.70	107.35	71.57	15.56	15.44	15.24	
Si ( $322 \pm 5.67$ ) [g/kg]											
85	1.3	42.4*	4.20	9.91	-98.55	-49.27	-32.85	55.16	39.60	29.46	
64	1.1	270.7	12.00	4.43	-18.08	-9.04	-6.03	4.16	3.86	3.49	
77	1.0	289	1.50	0.52	-11.63	-5.82	-3.88	10.28	5.62	3.82	
63	1.2	291.68	32.86	11.27	-10.69	-5.34	-3.56	0.92	0.91	0.89	
69	1.1	296	15.50	5.24	-9.16	-4.58	-3.05	1.65	1.58	1.47	
87	1.3	297.08	11.04	3.72	-8.78	-4.39	-2.93	2.19	2.01	1.79	
76	1.3	304.48	8.54	2.81	-6.17	-3.09	-2.06	1.95	1.71	1.45	
58	1.0	309.2	1.80	0.58	-4.51	-2.26	-1.50	3.81	2.15	1.47	
37	1.2	311.47	0.38	0.12	-3.71	-1.86	-1.24	3.68	1.85	1.24	
55	1.2	316.41	0.82	0.26	-1.97	-0.98	-0.66	1.89	0.97	0.65	
88	1.0	316.7	22.00	6.95	-1.87	-0.93	-0.62	0.24	0.23	0.22	
74	2.0	317.85	0.0005	2E-04	-1.46	-0.73	-0.49	1.46	0.73	0.49	
86	1.2	321.72	1.58	0.49	-0.10	-0.05	-0.03	0.09	0.05	0.03	
21	2.0	330.18	4.04	1.22	2.88	1.44	0.96	1.66	1.17	0.87	
70	1.2	522.54*	68.29	13.07	70.68	35.34	23.56	2.93	2.93	2.91	
73	1.0	535.38*	2.29	0.43	75.21	37.60	25.07	58.52	34.87	24.21	
68	1.3	610.82*	4.56	0.75	101.80	50.90	33.93	53.76	39.67	29.91	
Ti ( $4.300 \pm 0.20$ ) [g/kg]											
4	1.1	1.89*	0.38	20.00	-24.68	-12.34	-8.23	6.17	5.66	5.04	
84	1.2	2.57	0.16	6.18	-17.68	-8.84	-5.89	9.25	6.85	5.18	
54	1.0	2.99	0.19	6.31	-13.39	-6.69	-4.46	6.14	4.81	3.75	
37	1.2	3.46	0.02	0.56	-8.60	-4.30	-2.87	8.44	4.28	2.86	
71	1.1	3.79	0.95	25.21	-5.27	-2.63	-1.76	0.54	0.53	0.51	
78	1.1	3.86	0.003	0.08	-4.41	-2.21	-1.47	4.41	2.20	1.47	
88	1.0	3.89	0.34	8.74	-4.23	-2.12	-1.41	1.17	1.06	0.92	

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED *z*- AND *u*-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	<i>z</i> -scores			<i>u</i> -scores			<i>k</i> = 1.5
					<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	<i>k</i> = 0.5	<i>k</i> = 1.0		
77	1.0	3.9	0.21	5.38	-4.10	-2.05	-1.37	1.73	1.39	1.11	
55	5.0	3.97	0.58	14.70	-3.37	-1.69	-1.12	0.56	0.54	0.50	
72	1.4	4.02	0.07	1.72	-2.90	-1.45	-0.97	2.36	1.36	0.94	
69	1.1	4.05	0.22	5.31	-2.56	-1.28	-0.85	1.06	0.86	0.69	
53	2.0	4.06	0.40	9.85	-2.46	-1.23	-0.82	0.58	0.54	0.48	
79	1.3	4.16	0.07	1.59	-1.41	-0.71	-0.47	1.17	0.67	0.46	
15	1.3	4.22	0.30	7.11	-0.82	-0.41	-0.27	0.25	0.22	0.19	
74	2.0	4.26	0.01	0.15	-0.39	-0.19	-0.13	0.39	0.19	0.13	
62	1.3	4.3	0.44	10.26	0.00	0.00	0.00	0.00	0.00	0.00	
58	1.0	4.38	0.06	1.33	0.77	0.38	0.26	0.66	0.37	0.25	
21	2.0	4.42	0.16	3.65	1.19	0.59	0.40	0.62	0.46	0.35	
57	1.4	4.42	0.07	1.49	1.24	0.62	0.41	1.03	0.59	0.40	
64	1.1	4.55	0.10	2.20	2.56	1.28	0.85	1.79	1.14	0.81	
87	1.3	4.73	0.01	0.23	4.36	2.18	1.45	4.33	2.18	1.45	
70	1.2	5.01	0.16	3.25	7.23	3.61	2.41	3.72	2.78	2.11	
86	1.2	5.03	0.04	0.89	7.45	3.72	2.48	6.77	3.63	2.45	
56	1.3	5.15	0.25	4.86	8.66	4.33	2.89	3.15	2.67	2.20	
63	1.2	5.16	0.12	2.27	8.79	4.39	2.93	5.63	3.77	2.72	
76	1.3	5.2	0.15	2.92	9.19	4.60	3.06	4.97	3.63	2.72	
85	1.3	6.12	0.65	10.62	18.64	9.32	6.21	2.77	2.68	2.55	
59	1.2	6.53	0.11	1.61	22.85	11.42	7.62	15.56	10.06	7.17	
68	1.3	11.31*	0.24	2.10	71.79	35.89	23.93	27.28	22.78	18.58	
73	1.0	15.99*	0.16	0.97	119.71	59.85	39.90	63.80	46.88	35.27	

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED z- AND u-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	z-scores			u-scores		
					k = 0.5	k = 1.0	k = 1.5	k = 0.5	k = 1.0	k = 1.5
As ( $13.40 \pm 1.45$ ) [mg/kg]										
57	1.4	7.2	1.50	20.83	-8.55	-4.27	-2.85	3.72	2.97	2.35
15	1.3	9.4	4.30	45.74	-5.52	-2.76	-1.84	0.92	0.88	0.83
74	2.0	10.6	0.71	6.70	-3.86	-1.93	-1.29	2.76	1.73	1.22
37	1.2	11.966	0.29	2.44	-1.98	-0.99	-0.66	1.83	0.97	0.65
82	1.2	12.125	0.33	2.69	-1.76	-0.88	-0.59	1.60	0.86	0.58
56	1.3	12.9	0.60	4.65	-0.69	-0.34	-0.23	0.53	0.32	0.22
21	2.0	13.4	0.74	5.52	0.00	0.00	0.00	0.00	0.00	0.00
55	5.0	13.739	0.93	6.80	0.47	0.23	0.16	0.29	0.20	0.14
79	1.3	14	1.36	9.69	0.83	0.41	0.28	0.39	0.30	0.23
61	5.0	15.77	0.42	2.66	3.27	1.63	1.09	2.83	1.57	1.07
84	1.2	15.85	3.20	20.19	3.38	1.69	1.13	0.75	0.70	0.63
85	1.3	16.3	1.30	7.98	4.00	2.00	1.33	1.95	1.49	1.14
58	1.0	18.81	0.71	3.77	7.46	3.73	2.49	5.33	3.35	2.36
69	1.1	19.8	4.40	22.22	8.82	4.41	2.94	1.44	1.38	1.30
87	1.3	30.439*	7.61	25.00	23.49	11.75	7.83	2.23	2.20	2.15
68	1.3	76.64*	2.14	2.79	87.20	43.60	29.07	27.99	24.46	20.72
Ba ( $410 \pm 26.52$ ) [mg/kg]										
87	1.3	374.111	0.94	0.25	-2.71	-1.35	-0.90	2.70	1.35	0.90
74	2.0	403.94	7.74	1.92	-0.46	-0.23	-0.15	0.39	0.22	0.15
61	5.0	404	50.00	12.38	-0.45	-0.23	-0.15	0.12	0.11	0.09
56	1.3	422	25.00	5.92	0.90	0.45	0.30	0.42	0.33	0.26
37	1.2	425.952	11.31	2.66	1.20	0.60	0.40	0.92	0.55	0.39
55	5.0	428.16	94.19	22.00	1.37	0.68	0.46	0.19	0.19	0.18
63	1.2	433	28.00	6.47	1.73	0.87	0.58	0.74	0.60	0.47
69	1.1	437	33.00	7.55	2.04	1.02	0.68	0.76	0.64	0.52
79	1.3	438	11.92	2.72	2.11	1.06	0.70	1.57	0.96	0.67
71	1.1	442.17	101.57	22.97	2.43	1.21	0.81	0.31	0.31	0.29
76	1.3	443.15	16.73	3.78	2.50	1.25	0.83	1.55	1.06	0.77
85	1.3	474	47.00	9.92	4.83	2.41	1.61	1.31	1.19	1.04
64	1.1	530*	25.00	4.72	9.05	4.52	3.02	4.24	3.29	2.55
73	1.0	7108.083*	477.22	6.71	505.12	252.56	168.37	14.03	14.01	13.99
Bi [mg/kg]										
68	1.3	14.84	1.70	11.46	-	-	-	-	-	-
Br ( $8.39 \pm 0.97$ ) [mg/kg]										
63	1.2	4.5	1.20	26.67	-7.98	-3.99	-2.66	3.00	2.52	2.06
77	1.0	5	1.00	20.00	-6.96	-3.48	-2.32	3.05	2.43	1.91
37	1.2	6.84	0.08	1.13	-3.18	-1.59	-1.06	3.14	1.59	1.06
84	1.2	6.849	1.30	18.98	-3.16	-1.58	-1.05	1.11	0.95	0.79
85	1.3	7.55	0.10	1.32	-1.72	-0.86	-0.57	1.69	0.86	0.57
69	1.1	8.1	0.70	8.64	-0.60	-0.30	-0.20	0.34	0.24	0.18

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED *z*- AND *u*-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	<i>z</i> -scores			<i>u</i> -scores		
					<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5
55	5.0	8.921	0.28	3.19	1.09	0.54	0.36	0.94	0.52	0.36
88	1.0	8.93	1.24	13.89	1.11	0.55	0.37	0.41	0.34	0.28
15	1.3	9	1.30	14.44	1.25	0.63	0.42	0.44	0.38	0.31
54	1.0	9.92	1.19	12.00	3.14	1.57	1.05	1.19	0.99	0.81
87	1.3	10.138	0.17	1.67	3.59	1.79	1.20	3.39	1.77	1.19
56	1.3	10.4	0.50	4.81	4.13	2.06	1.38	2.88	1.84	1.30
76	1.3	10.71	0.75	7.00	4.76	2.38	1.59	2.59	1.89	1.41
82	1.2	22.6*	0.57	2.50	29.16	14.58	9.72	19.03	12.61	9.07
Cd ( $0.503 \pm 0.09$ ) [mg/kg]										
37	1.2	0.47	0.16	34.47	-0.74	-0.37	-0.25	0.20	0.18	0.16
87	1.3	0.549	0.04	7.84	1.03	0.52	0.34	0.74	0.46	0.33
69	1.1	3.3*	0.33	10.00	62.69	31.35	20.90	8.40	8.18	7.85
Ce ( $73.3 \pm 6.14$ ) [mg/kg]										
87	1.3	61.263	0.55	0.90	-3.92	-1.96	-1.31	3.86	1.95	1.30
74	2.0	62	7.69	12.40	-3.68	-1.84	-1.23	1.36	1.15	0.94
69	1.1	70.4	5.40	7.67	-0.94	-0.47	-0.31	0.47	0.35	0.27
55	5.0	78.335	1.96	2.50	1.64	0.82	0.55	1.38	0.78	0.53
64	1.1	80	6.00	7.50	2.18	1.09	0.73	0.99	0.78	0.61
71	1.1	80.46	16.04	19.94	2.33	1.17	0.78	0.44	0.42	0.39
61	5.0	85.01	0.94	1.11	3.81	1.91	1.27	3.65	1.88	1.26
79	1.3	85.12	3.37	3.96	3.85	1.92	1.28	2.59	1.69	1.20
76	1.3	86.52	2.98	3.44	4.30	2.15	1.43	3.09	1.94	1.36
85	1.3	93	9.00	9.68	6.41	3.21	2.14	2.07	1.81	1.53
Cl [mg/kg]										
68	1.3	180.45	6.79	3.76	-	-	-	-	-	-
70	1.2	490.8	148.00	30.15	-	-	-	-	-	-
64	1.1	1400	200.00	14.29	-	-	-	-	-	-
Co ( $12.50 \pm 1.37$ ) [mg/kg]										
87	1.3	6.859	0.37	5.33	-8.25	-4.13	-2.75	7.28	3.99	2.71
58	1.0	8.23	0.28	3.40	-6.25	-3.12	-2.08	5.78	3.06	2.06
63	1.2	9.99	1.35	13.51	-3.67	-1.84	-1.22	1.66	1.31	1.02
74	2.0	11.4	3.76	32.98	-1.61	-0.80	-0.54	0.29	0.27	0.26
85	1.3	11.5	1.10	9.57	-1.46	-0.73	-0.49	0.77	0.57	0.43
55	5.0	11.79	0.19	1.60	-1.04	-0.52	-0.35	1.00	0.51	0.34
21	2.0	12	0.37	3.08	-0.73	-0.37	-0.24	0.64	0.35	0.24
61	5.0	13.49	0.19	1.41	1.45	0.72	0.48	1.40	0.72	0.48
57	1.4	34.4*	4.10	11.92	32.03	16.02	10.68	5.27	5.07	4.78
84	1.2	59.37*	12.00	20.21	68.56	34.28	22.85	3.90	3.88	3.85
62	1.3	179.49*	16.50	9.19	244.27	122.13	81.42	10.11	10.09	10.04

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED z- AND u-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	z-scores			u-scores		
					k = 0.5	k = 1.0	k = 1.5	k = 0.5	k = 1.0	k = 1.5
Cr ( $89.6 \pm 7.29$ ) [mg/kg]										
77	1.0	32	3.50	10.94	-15.81	-7.91	-5.27	11.40	7.13	5.02
37	1.2	34.407	1.01	2.93	-15.15	-7.57	-5.05	14.60	7.50	5.03
84	1.2	42.67	8.60	20.15	-12.88	-6.44	-4.29	5.02	4.16	3.37
72	1.4	69.937	2.02	2.89	-5.40	-2.70	-1.80	4.72	2.60	1.77
53	1.4	72	3.00	4.17	-4.83	-2.42	-1.61	3.73	2.23	1.55
15	1.3	76	39.00	51.32	-3.73	-1.87	-1.24	0.35	0.34	0.34
57	1.4	83.9	3.90	4.65	-1.56	-0.78	-0.52	1.07	0.69	0.49
74	2.0	86	4.05	4.72	-0.99	-0.49	-0.33	0.66	0.43	0.31
21	2.0	89.1	2.87	3.22	-0.14	-0.07	-0.05	0.11	0.06	0.04
79	1.3	92.4	1.14	1.23	0.77	0.38	0.26	0.73	0.38	0.25
55	5.0	93.64	4.03	4.30	1.11	0.55	0.37	0.74	0.49	0.35
58	1.0	96.1	8.00	8.32	1.78	0.89	0.59	0.74	0.60	0.48
64	1.1	105	5.00	4.76	4.23	2.11	1.41	2.49	1.74	1.28
61	5.0	105.8	2.80	2.65	4.45	2.22	1.48	3.53	2.08	1.44
87	1.3	111.021	0.31	0.28	5.88	2.94	1.96	5.86	2.94	1.96
76	1.3	127.79	17.21	13.47	10.48	5.24	3.49	2.17	2.04	1.87
70	1.2	129.5	33.50	25.87	10.95	5.48	3.65	1.18	1.16	1.13
63	1.2	130	14.00	10.77	11.09	5.54	3.70	2.79	2.56	2.27
88	1.0	130.67	25.51	19.52	11.27	5.64	3.76	1.59	1.55	1.48
69	1.1	131	19.00	14.50	11.36	5.68	3.79	2.14	2.03	1.89
68	1.3	495.14*	24.61	4.97	111.31	55.66	37.10	16.30	15.80	15.06
85	1.3	1004*	100.00	9.96	250.99	125.49	83.66	9.14	9.12	9.09
Cs [mg/kg]										
55	5.0	6.895*	0.23	3.40	-	-	-	-	-	-
64	1.1	8	2.00	25.00	-	-	-	-	-	-
61	5.0	8.18	0.39	4.77	-	-	-	-	-	-
87	1.3	9.006	0.68	7.59	-	-	-	-	-	-
Cu ( $20.1 \pm 2.05$ ) [mg/kg]										
4	1.1	7.1	1.40	19.72	-12.70	-6.35	-4.23	7.50	5.24	3.85
15	1.3	14	5.60	40.00	-5.96	-2.98	-1.99	1.07	1.02	0.96
62	1.3	14.126	1.48	10.48	-5.84	-2.92	-1.95	3.32	2.36	1.75
72	1.4	15.827	1.67	10.58	-4.18	-2.09	-1.39	2.18	1.62	1.22
78	1.1	16	5.00	31.25	-4.01	-2.00	-1.34	0.80	0.76	0.70
37	1.2	17.352	0.43	2.50	-2.69	-1.34	-0.90	2.47	1.31	0.89
63	1.2	18.48	3.65	19.75	-1.58	-0.79	-0.53	0.43	0.39	0.34
55	1.2	19.149	2.50	13.06	-0.93	-0.46	-0.31	0.35	0.29	0.24
56	1.3	19.3	1.20	6.22	-0.78	-0.39	-0.26	0.51	0.34	0.24
74	2.0	20	4.26	21.30	-0.10	-0.05	-0.03	0.02	0.02	0.02
64	1.1	20	3.00	15.00	-0.10	-0.05	-0.03	0.03	0.03	0.02
21	2.0	20.4	0.60	2.94	0.29	0.15	0.10	0.25	0.14	0.10
77	1.0	23	4.20	18.26	2.83	1.42	0.94	0.67	0.62	0.56

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED *z*- AND *u*-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	<i>z</i> -scores			<i>u</i> -scores		
					<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5
84	1.2	23.68	4.10	17.31	3.50	1.75	1.17	0.85	0.78	0.70
79	1.3	24.4	1.34	5.50	4.20	2.10	1.40	2.55	1.76	1.28
86	1.2	24.74	0.45	1.82	4.53	2.27	1.51	4.15	2.21	1.50
58	1.0	25.2	2.90	11.51	4.98	2.49	1.66	1.66	1.44	1.21
70	1.2	29.97	20.72	69.14	9.64	4.82	3.21	0.48	0.47	0.47
57	1.4	31	1.60	5.16	10.65	5.33	3.55	5.74	4.20	3.15
85	1.3	36	4.00	11.11	15.54	7.77	5.18	3.85	3.54	3.15
88	1.0	40.3	4.93	12.23	19.74	9.87	6.58	4.01	3.78	3.48
69	1.1	48.6*	4.00	8.23	27.85	13.92	9.28	6.90	6.34	5.65
82	1.2	54.75*	1.77	3.23	33.86	16.93	11.29	16.95	12.81	9.78
87	1.3	57.632*	0.42	0.73	36.67	18.34	12.22	33.89	17.96	12.11
68	1.3	103.51*	6.53	6.31	81.50	40.75	27.17	12.62	12.19	11.56
76	1.3	252.8*	9.12	3.61	227.37	113.68	75.79	25.36	24.90	24.18
Dy [mg/kg]										
87	1.3	4.58	1.43	31.15	-	-	-	-	-	-
55	5.0	6.789	0.48	7.10	-	-	-	-	-	-
Er [mg/kg]										
87	1.3	2.918	0.29	9.89	-	-	-	-	-	-
Eu [mg/kg]										
55	5.0	1.281	0.09	7.10	-	-	-	-	-	-
61	5.0	1.393	0.05	3.30	-	-	-	-	-	-
Ga (13.6 ± 0.73) [mg/kg]										
84	1.2	7.971	1.50	18.82	-7.66	-3.83	-2.55	3.37	2.68	2.11
72	1.4	8.415	0.63	7.43	-7.06	-3.53	-2.35	5.38	3.25	2.26
74	2.0	10.4	0.44	4.28	-4.36	-2.18	-1.45	3.73	2.09	1.42
88	1.0	10.93	2.15	19.67	-3.64	-1.82	-1.21	1.18	1.03	0.87
78	1.1	11	6.00	54.55	-3.54	-1.77	-1.18	0.43	0.42	0.41
63	1.2	11.2	1.60	14.29	-3.27	-1.63	-1.09	1.36	1.10	0.88
62	1.3	11.937	1.34	11.20	-2.26	-1.13	-0.75	1.09	0.84	0.65
69	1.1	12.4	1.60	12.90	-1.63	-0.82	-0.54	0.68	0.55	0.44
54	1.0	12.5	2.50	20.00	-1.50	-0.75	-0.50	0.42	0.38	0.33
15	1.3	12.5	2.10	16.80	-1.50	-0.75	-0.50	0.49	0.43	0.36
37	1.2	12.908	0.30	2.31	-0.94	-0.47	-0.31	0.87	0.46	0.31
79	1.3	15	1.00	6.67	1.91	0.95	0.64	1.13	0.79	0.58
56	1.3	15.1	0.60	3.97	2.04	1.02	0.68	1.58	0.95	0.66
76	1.3	15.14	0.55	3.63	2.10	1.05	0.70	1.68	0.98	0.68
85	1.3	18	2.00	11.11	5.99	3.00	2.00	2.07	1.77	1.48
87	1.3	19.402	0.81	4.19	7.90	3.95	2.63	5.30	3.46	2.47
82	1.2	59.425*	1.50	2.52	62.40	31.20	20.80	27.50	21.86	17.21
Ge [mg/kg]										
87	1.3	1.989	0.26	13.00	-	-	-	-	-	-

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED z- AND u-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	z-scores			u-scores		
					k = 0.5	k = 1.0	k = 1.5	k = 0.5	k = 1.0	k = 1.5
74	2.0	3.47	0.27	7.78	-	-	-	-	-	-
Hf [mg/kg]										
85	1.3	6	0.80	13.33	-	-	-	-	-	-
55	5.0	7	0.27	3.80	-	-	-	-	-	-
87	1.3	7.36	1.47	20.00	-	-	-	-	-	-
61	5.0	8.84	0.28	3.17	-	-	-	-	-	-
Hg (0.05 ± 0.01) [mg/kg]										
68	1.3	3.19	1.58	49.53	570.91	285.45	190.30	1.99	1.99	1.99
Ho [mg/kg]										
87	1.3	1.001	0.29	28.83	-	-	-	-	-	-
I [mg/kg]										
64	1.1	2	2.00	100.0	-	-	-	-	-	-
87	1.3	5.279	0.46	8.69	-	-	-	-	-	-
69	1.1	8.1	0.70	8.64	-	-	-	-	-	-
La (36.1 ± 3.37) [mg/kg]										
64	1.1	27	3.00	11.11	-5.41	-2.70	-1.80	2.65	2.02	1.55
69	1.1	30.1	2.30	7.64	-3.56	-1.78	-1.19	2.11	1.47	1.08
87	1.3	32.933	0.23	0.69	-1.88	-0.94	-0.63	1.86	0.94	0.63
21	2.0	33.9	2.70	7.96	-1.31	-0.65	-0.44	0.69	0.51	0.38
74	2.0	37	0.89	2.41	0.53	0.27	0.18	0.47	0.26	0.18
71	1.1	39.09	8.15	20.85	1.78	0.89	0.59	0.36	0.34	0.31
55	5.0	39.81	0.28	0.70	2.20	1.10	0.73	2.17	1.10	0.73
86	1.2	39.81	1.03	2.59	2.20	1.10	0.73	1.88	1.05	0.72
79	1.3	40.58	3.44	8.48	2.66	1.33	0.89	1.17	0.93	0.73
61	5.0	41.46	0.74	1.78	3.18	1.59	1.06	2.92	1.56	1.05
37	1.2	41.739	4.50	10.78	3.35	1.68	1.12	1.17	1.00	0.83
85	1.3	42	5.00	11.90	3.51	1.75	1.17	1.12	0.98	0.83
76	1.3	43.33	2.00	4.62	4.30	2.15	1.43	2.77	1.85	1.33
Lu [mg/kg]										
55	5.0	0.193	0.03	15.62	-	-	-	-	-	-
87	1.3	0.443	0.01	1.87	-	-	-	-	-	-
61	5.0	0.573	0.02	4.19	-	-	-	-	-	-
Mo [mg/kg]										
87	1.3	1.063	0.10	8.98	-	-	-	-	-	-
63	1.2	1.98	0.71	35.86	-	-	-	-	-	-
68	1.3	19.51*	0.98	5.02	-	-	-	-	-	-
Nb (16.0 ± 1.69) [mg/kg]										
4	1.1	10.7	3.90	36.45	-6.29	-3.14	-2.10	1.33	1.25	1.14

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED *z*- AND *u*-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	<i>z</i> -scores			<i>u</i> -scores		
					<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5
54	1.0	11.9	1.40	11.76	-4.86	-2.43	-1.62	2.51	1.87	1.42
69	1.1	12.5	0.75	6.00	-4.15	-2.08	-1.38	3.10	1.90	1.33
56	1.3	13.8	0.50	3.62	-2.61	-1.30	-0.87	2.24	1.25	0.85
63	1.2	14.21	2.02	14.22	-2.12	-1.06	-0.71	0.82	0.68	0.55
87	1.3	16.082	0.24	1.47	0.10	0.05	0.03	0.09	0.05	0.03
74	2.0	16.1	2.31	14.35	0.12	0.06	0.04	0.04	0.03	0.03
21	2.0	16.4	0.30	1.83	0.47	0.24	0.16	0.45	0.23	0.16
24	1.1	16.965	2.20	12.96	1.14	0.57	0.38	0.41	0.35	0.29
85	1.3	24*	2.00	8.33	9.49	4.74	3.16	3.69	3.06	2.48
68	1.3	41.42*	0.83	2.00	30.15	15.07	10.05	21.49	13.53	9.55
Nd ( $32.7 \pm 3.09$ ) [mg/kg]										
87	1.3	26.771	1.11	4.15	-3.83	-1.92	-1.28	3.11	1.80	1.24
69	1.1	32.6	2.60	7.98	-0.06	-0.03	-0.02	0.03	0.02	0.02
85	1.3	39	4.00	10.26	4.07	2.04	1.36	1.47	1.25	1.03
71	1.1	40.68	11.54	28.37	5.16	2.58	1.72	0.69	0.67	0.64
79	1.3	44.48	0.92	2.08	7.61	3.81	2.54	6.54	3.65	2.49
Ni ( $37.9 \pm 3.51$ ) [mg/kg]										
82	1.2	10.625	0.28	2.59	-15.55	-7.77	-5.18	15.36	7.75	5.18
87	1.3	15.548	0.15	0.96	-12.74	-6.37	-4.25	12.70	6.37	4.25
70	1.2	20.22	23.10	114.2	-10.08	-5.04	-3.36	0.76	0.76	0.75
63	1.2	24.48	3.60	14.71	-7.65	-3.83	-2.55	3.35	2.67	2.10
78	1.1	26	3.00	11.54	-6.78	-3.39	-2.26	3.42	2.58	1.96
84	1.2	26.64	2.80	10.51	-6.42	-3.21	-2.14	3.41	2.51	1.89
64	1.1	30	2.00	6.67	-4.50	-2.25	-1.50	2.97	1.96	1.40
69	1.1	30.3	4.00	13.20	-4.33	-2.17	-1.44	1.74	1.43	1.15
88	1.0	33.9	5.71	16.84	-2.28	-1.14	-0.76	0.67	0.60	0.52
74	2.0	36	2.33	6.47	-1.08	-0.54	-0.36	0.65	0.45	0.33
77	1.0	38	3.20	8.42	0.06	0.03	0.02	0.03	0.02	0.02
15	1.3	39	6.40	16.41	0.63	0.31	0.21	0.17	0.15	0.13
37	1.2	39.486	0.77	1.94	0.90	0.45	0.30	0.83	0.44	0.30
21	2.0	39.6	0.79	1.99	0.97	0.48	0.32	0.88	0.47	0.32
72	1.4	42.555	1.74	4.08	2.65	1.33	0.88	1.89	1.19	0.84
57	1.4	44.5	2.60	5.84	3.76	1.88	1.25	2.10	1.51	1.12
56	1.3	48	3.00	6.25	5.76	2.88	1.92	2.91	2.19	1.67
79	1.3	49.2	4.02	8.18	6.44	3.22	2.15	2.57	2.12	1.71
76	1.3	59.46	6.75	11.35	12.29	6.15	4.10	3.09	2.83	2.52
85	1.3	65	6.00	9.23	15.45	7.72	5.15	4.34	3.90	3.40
68	1.3	230.97*	12.75	5.52	110.07	55.03	36.69	15.00	14.60	14.00
Pb ( $36.9 \pm 3.43$ ) [mg/kg]										
84	1.2	3.223	0.57	17.69	-19.64	-9.82	-6.55	18.64	9.69	6.51
87	1.3	9.711	0.04	0.42	-15.86	-7.93	-5.29	15.85	7.93	5.29
68	1.3	11.24	2.40	21.35	-14.96	-7.48	-4.99	8.70	6.13	4.52

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED z- AND u-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	z-scores			u-scores		
					k = 0.5	k = 1.0	k = 1.5	k = 0.5	k = 1.0	k = 1.5
86	1.2	19.37	0.42	2.17	-10.22	-5.11	-3.41	9.93	5.07	3.40
82	1.2	25.5	0.68	2.68	-6.65	-3.32	-2.22	6.18	3.26	2.20
57	1.4	29.2	3.50	11.99	-4.49	-2.25	-1.50	1.98	1.57	1.24
69	1.1	30.1	8.00	26.58	-3.97	-1.98	-1.32	0.83	0.78	0.71
63	1.2	31.47	3.20	10.17	-3.17	-1.58	-1.06	1.50	1.16	0.90
55	1.2	33.481	1.53	4.57	-1.99	-1.00	-0.66	1.49	0.91	0.64
37	1.2	34.162	0.37	1.09	-1.60	-0.80	-0.53	1.56	0.79	0.53
74	2.0	35.3	2.22	6.30	-0.93	-0.47	-0.31	0.57	0.39	0.29
56	1.3	35.4	1.50	4.24	-0.87	-0.44	-0.29	0.66	0.40	0.28
53	1.4	36	2.00	5.56	-0.52	-0.26	-0.17	0.34	0.23	0.16
21	2.0	37	1.12	3.03	0.06	0.03	0.02	0.05	0.03	0.02
54	1.0	41.4	3.20	7.73	2.62	1.31	0.87	1.24	0.96	0.74
79	1.3	42.2	3.56	8.44	3.09	1.55	1.03	1.34	1.07	0.85
15	1.3	43.7	13.20	30.21	3.97	1.98	1.32	0.51	0.50	0.48
72	1.4	43.877	1.23	2.80	4.07	2.03	1.36	3.31	1.92	1.32
85	1.3	48	4.00	8.33	6.47	3.24	2.16	2.55	2.11	1.70
78	1.1	48	2.00	4.17	6.47	3.24	2.16	4.21	2.80	2.01
64	1.1	53	4.00	7.55	9.39	4.69	3.13	3.70	3.06	2.47
76	1.3	55.72	6.68	11.99	10.98	5.49	3.66	2.73	2.51	2.23
88	1.0	56.83	5.25	9.24	11.62	5.81	3.87	3.61	3.18	2.71
77	1.0	59	4.30	7.29	12.89	6.44	4.30	4.77	4.02	3.30
62	1.3	66.406	5.42	8.16	17.21	8.60	5.74	5.19	4.60	3.95
70	1.2	420.1*	172.80	41.13	223.48	111.74	74.49	2.22	2.22	2.22
					Pr [mg/kg]					
87	1.3	7.905	0.05	0.60	-	-	-	-	-	-
					Rb (107 ± 8.47) [mg/kg]					
82	1.2	4.7*	0.12	2.55	-24.15	-12.07	-8.05	24.14	12.07	8.05
57	1.4	7.4*	1.20	16.22	-23.51	-11.76	-7.84	22.62	11.64	7.80
63	1.2	37.6	2.80	7.45	-16.38	-8.19	-5.46	13.67	7.78	5.33
53	1.4	44	2.00	4.55	-14.87	-7.44	-4.96	13.45	7.24	4.90
84	1.2	45.79	4.80	10.48	-14.45	-7.22	-4.82	9.56	6.29	4.51
4	1.1	73.1	8.30	11.35	-8.00	-4.00	-2.67	3.64	2.86	2.23
54	1.0	91.4	3.20	3.50	-3.68	-1.84	-1.23	2.94	1.72	1.19
74	2.0	99	2.22	2.24	-1.89	-0.94	-0.63	1.67	0.91	0.62
72	1.4	100.555	3.09	3.08	-1.52	-0.76	-0.51	1.23	0.71	0.49
56	1.3	102.3	5.00	4.89	-1.11	-0.55	-0.37	0.72	0.48	0.34
69	1.1	105	6.00	5.71	-0.47	-0.24	-0.16	0.27	0.19	0.14
55	1.2	106.152	2.54	2.40	-0.20	-0.10	-0.07	0.17	0.10	0.07
59	1.2	109	18.00	16.51	0.47	0.24	0.16	0.11	0.10	0.09
64	1.1	109	5.00	4.59	0.47	0.24	0.16	0.31	0.20	0.15
15	1.3	109.3	7.20	6.59	0.54	0.27	0.18	0.28	0.21	0.16
88	1.0	110.33	9.31	8.44	0.79	0.39	0.26	0.33	0.26	0.21
85	1.3	111	14.00	12.61	0.94	0.47	0.31	0.27	0.24	0.21

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED *z*- AND *u*-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	<i>z</i> -scores			<i>u</i> -scores		
					<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5
21	2.0	111	1.83	1.65	0.94	0.47	0.31	0.87	0.46	0.31
37	1.2	111.231	0.36	0.33	1.00	0.50	0.33	1.00	0.50	0.33
87	1.3	111.263	0.54	0.49	1.01	0.50	0.34	1.00	0.50	0.34
77	1.0	113	8.50	7.52	1.42	0.71	0.47	0.63	0.50	0.39
61	5.0	118.2	8.40	7.11	2.64	1.32	0.88	1.19	0.94	0.74
24	1.1	119.528	11.78	9.85	2.96	1.48	0.99	1.00	0.86	0.72
79	1.3	123.8	1.92	1.55	3.97	1.98	1.32	3.61	1.93	1.31
76	1.3	132.81	5.44	4.10	6.09	3.05	2.03	3.74	2.56	1.87
71	1.1	134.25	34.52	25.71	6.43	3.22	2.14	0.78	0.77	0.74
62	1.3	145.981	1.05	0.72	9.20	4.60	3.07	8.93	4.57	3.06
68	1.3	170.3	1.58	0.93	14.94	7.47	4.98	14.00	7.34	4.94
70	1.2	373.7*	125.60	33.61	62.96	31.48	20.99	2.12	2.12	2.11
73	1.0	1710.185*	197.75	11.56	378.46	189.23	126.15	8.11	8.10	8.09
S ( $328 \pm 21.94$ ) [mg/kg]										
56	1.3	244	12.00	4.92	-7.66	-3.83	-2.55	5.17	3.36	2.40
79	1.3	247.8	23.21	9.37	-7.31	-3.66	-2.44	3.12	2.51	1.99
69	1.1	289	62.00	21.45	-3.55	-1.78	-1.18	0.62	0.59	0.56
87	1.3	460	26.54	5.77	12.03	6.02	4.01	4.60	3.83	3.12
37	1.2	523.655	6.52	1.24	17.83	8.92	5.94	15.33	8.55	5.83
55	1.2	585.906	10.66	1.82	23.51	11.75	7.84	16.86	10.57	7.46
70	1.2	1025.9	337.60	32.91	63.61	31.81	21.20	2.07	2.06	2.06
85	1.3	1076	108.00	10.04	68.18	34.09	22.73	6.89	6.79	6.63
68	1.3	1229.66	61.77	5.02	82.19	41.09	27.40	14.37	13.76	12.88
76	1.3	2132*	152.25	7.14	164.44	82.22	54.81	11.82	11.73	11.58
63	1.2	2539*	350.00	13.78	201.54	100.77	67.18	6.31	6.30	6.29
73	1.0	3180.165*	132.16	4.16	259.98	129.99	86.66	21.51	21.29	20.94
58	1.0	4510*	170.00	3.77	381.20	190.60	127.07	24.55	24.40	24.15
Sb ( $1.07 \pm 0.17$ ) [mg/kg]										
62	1.3	0.472*	0.03	6.57	-7.06	-3.53	-2.35	6.63	3.47	2.34
87	1.3	0.912	0.12	13.69	-1.87	-0.93	-0.62	1.05	0.75	0.56
61	5.0	1.186	0.05	4.55	1.37	0.68	0.46	1.15	0.65	0.45
55	5.0	1.22	0.19	15.58	1.77	0.88	0.59	0.72	0.59	0.47
Sc ( $10.2 \pm 1.15$ ) [mg/kg]										
68	1.3	6.79*	0.84	12.37	-5.93	-2.96	-1.98	3.35	2.39	1.78
21	2.0	9.8	0.44	4.49	-0.70	-0.35	-0.23	0.55	0.32	0.22
55	5.0	9.848	0.03	0.30	-0.61	-0.31	-0.20	0.61	0.31	0.20
61	5.0	10.53*	0.20	1.90	0.57	0.29	0.19	0.54	0.28	0.19
87	1.3	25.125*	1.49	5.95	25.95	12.97	8.65	9.32	7.92	6.54
Se [mg/kg]										
68	1.3	3.47	0.73	21.04	-	-	-	-	-	-

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED z- AND u-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	z-scores			u-scores		
					k = 0.5	k = 1.0	k = 1.5	k = 0.5	k = 1.0	k = 1.5
Sm [mg/kg]										
87	1.3	5.19	1.22	23.49	-	-	-	-	-	-
55	5.0	6.663	0.03	0.41	-	-	-	-	-	-
61	5.0	7.68	0.12	1.56	-	-	-	-	-	-
Sn ( $3.68 \pm 0.48$ ) [mg/kg]										
87	1.3	2.992	0.05	1.77	-2.84	-1.42	-0.95	2.78	1.41	0.95
79	1.3	4.12	0.04	1.09	1.82	0.91	0.61	1.79	0.91	0.61
68	1.3	11.56	4.73	40.92	32.57	16.29	10.86	1.66	1.66	1.65
64	1.1	18	2.00	11.11	59.19	29.60	19.73	7.11	6.96	6.73
Sr ( $106 \pm 8.40$ ) [mg/kg]										
82	1.2	7.85*	0.20	2.51	-23.36	-11.68	-7.79	23.33	11.67	7.78
53	1.4	36*	2.00	5.56	-16.66	-8.33	-5.55	15.04	8.10	5.48
57	1.4	69.7	1.80	2.58	-8.64	-4.32	-2.88	7.94	4.22	2.85
4	1.1	74.6	8.40	11.26	-7.47	-3.74	-2.49	3.34	2.64	2.07
84	1.2	78.64	5.90	7.50	-6.51	-3.26	-2.17	3.78	2.66	1.97
54	1.0	83.7	2.10	2.51	-5.31	-2.65	-1.77	4.75	2.57	1.74
72	1.4	88.881	1.47	1.65	-4.07	-2.04	-1.36	3.85	2.01	1.35
79	1.1	97.392	3.04	3.12	-2.05	-1.02	-0.68	1.66	0.96	0.66
69	1.1	100	6.00	6.00	-1.43	-0.71	-0.48	0.82	0.58	0.43
55	1.2	101.303	1.68	1.66	-1.12	-0.56	-0.37	1.04	0.55	0.37
74	2.0	101.5	2.63	2.59	-1.07	-0.54	-0.36	0.91	0.51	0.35
15	1.3	101.5	6.60	6.50	-1.07	-0.54	-0.36	0.58	0.42	0.32
56	1.3	101.7	5.00	4.92	-1.02	-0.51	-0.34	0.66	0.44	0.32
63	1.2	102	14.00	13.73	-0.95	-0.48	-0.32	0.27	0.24	0.21
24	1.1	105.436	12.25	11.61	-0.13	-0.07	-0.04	0.04	0.04	0.03
87	1.3	106.597	0.67	0.63	0.14	0.07	0.05	0.14	0.07	0.05
21	2.0	107	1.52	1.42	0.24	0.12	0.08	0.22	0.12	0.08
37	1.2	107.214	0.54	0.50	0.29	0.14	0.10	0.29	0.14	0.10
88	1.0	108.67	9.18	8.45	0.64	0.32	0.21	0.26	0.21	0.17
59	1.2	110	19.00	17.27	0.95	0.48	0.32	0.21	0.19	0.18
62	1.3	116.366	10.52	9.04	2.47	1.23	0.82	0.92	0.77	0.63
85	1.3	119	10.00	8.40	3.09	1.55	1.03	1.20	1.00	0.81
71	1.1	119.89	28.28	23.59	3.31	1.65	1.10	0.49	0.47	0.45
77	1.0	120	7.20	6.00	3.33	1.67	1.11	1.68	1.27	0.96
76	1.3	122.69	6.53	5.32	3.97	1.99	1.32	2.15	1.57	1.18
64	1.1	150*	8.00	5.33	10.47	5.24	3.49	4.87	3.79	2.95
68	1.3	172.48*	1.38	0.80	15.82	7.91	5.27	15.03	7.81	5.24
70	1.2	428.6*	149.30	34.83	76.77	38.38	25.59	2.16	2.16	2.15
73	1.0	644.922*	11.70	1.81	128.24	64.12	42.75	43.36	37.42	31.34
Ta [mg/kg]										
70	1.2	266.7	157.30	58.98	-	-	-	-	-	-

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED *z*- AND *u*-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	<i>z</i> -scores			<i>u</i> -scores		
					<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5
Tb [mg/kg]										
87	1.3	0.909	0.25	27.97	-	-	-	-	-	-
61	5.0	1.23	0.19	15.45	-	-	-	-	-	-
Th (11.4 ± 1.26) [mg/kg]										
68	1.3	8.09	1.83	22.62	-5.24	-2.62	-1.75	1.71	1.49	1.26
69	1.1	8.8	0.80	9.09	-4.11	-2.06	-1.37	2.55	1.74	1.26
79	1.1	8.83	1.24	14.02	-4.07	-2.03	-1.36	1.85	1.45	1.13
77	1.0	9.6	0.60	6.25	-2.85	-1.42	-0.95	2.07	1.29	0.90
37	1.2	10.959	0.27	2.43	-0.70	-0.35	-0.23	0.64	0.34	0.23
74	2.0	11	2.21	20.09	-0.63	-0.32	-0.21	0.17	0.16	0.14
55	5.0	11.489	0.28	2.40	0.14	0.07	0.05	0.13	0.07	0.05
21	2.0	11.7	0.56	4.79	0.47	0.24	0.16	0.36	0.22	0.15
85	1.3	11.7	1.00	8.55	0.47	0.24	0.16	0.25	0.19	0.14
15	1.3	11.7	3.50	29.91	0.47	0.24	0.16	0.08	0.08	0.08
61	5.0	12.39	0.23	1.86	1.57	0.78	0.52	1.47	0.77	0.52
87	1.3	13.784	0.79	5.73	3.77	1.89	1.26	2.36	1.60	1.16
Tl (0.699 ± 0.12) [mg/kg]										
87	1.3	1.371	0.00	0.00	11.39	5.69	3.80	11.39	5.69	3.80
Tm [mg/kg]										
87	1.3	0.475	0.01	1.70	-	-	-	-	-	-
73	1.0	1710.185	197.75	11.56	-	-	-	-	-	-
U (2.74 ± 0.38) [mg/kg]										
85	1.3	2.1*	0.20	9.52	-3.40	-1.70	-1.13	2.33	1.50	1.07
55	5.0	2.2*	0.35	15.70	-2.87	-1.43	-0.96	1.37	1.06	0.82
37	1.2	3.006	0.71	23.72	1.41	0.71	0.47	0.36	0.33	0.29
61	5.0	3.03	0.22	7.26	1.54	0.77	0.51	1.00	0.66	0.48
21	2.0	3.36	0.25	7.44	3.29	1.65	1.10	1.98	1.37	1.00
68	1.3	18.9*	2.69	14.23	85.82	42.91	28.61	5.99	5.95	5.88
V (80.9 ± 6.68) [mg/kg]										
64	1.1	57	7.00	12.28	-7.15	-3.58	-2.38	3.08	2.47	1.96
77	1.0	58	4.20	7.24	-6.86	-3.43	-2.29	4.27	2.90	2.11
37	1.2	60.642	3.33	5.49	-6.06	-3.03	-2.02	4.29	2.71	1.92
63	1.2	69	12.00	17.39	-3.56	-1.78	-1.19	0.96	0.87	0.76
57	1.4	70.1	10.40	14.84	-3.23	-1.62	-1.08	0.99	0.87	0.75
58	1.0	77	4.60	5.97	-1.17	-0.58	-0.39	0.69	0.48	0.35
53	1.4	79	3.00	3.80	-0.57	-0.28	-0.19	0.42	0.26	0.18
21	2.0	79.5	1.18	1.48	-0.42	-0.21	-0.14	0.40	0.21	0.14
74	2.0	82	2.63	3.21	0.33	0.16	0.11	0.26	0.15	0.11
55	5.0	82.9	3.53	4.25	0.60	0.30	0.20	0.41	0.26	0.19

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED z- AND u-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	z-scores			u-scores		
					k = 0.5	k = 1.0	k = 1.5	k = 0.5	k = 1.0	k = 1.5
56	1.3	90	5.00	5.56	2.72	1.36	0.91	1.51	1.09	0.81
79	1.3	93.2	5.40	5.80	3.68	1.84	1.23	1.94	1.43	1.08
76	1.3	101.57	5.31	5.23	6.19	3.09	2.06	3.29	2.42	1.82
86	1.2	115.27	6.44	5.59	10.29	5.14	3.43	4.74	3.70	2.89
87	1.3	116.807	3.51	3.01	10.75	5.37	3.58	7.41	4.76	3.38
69	1.1	117	32.00	27.35	10.81	5.40	3.60	1.12	1.10	1.08
72	1.4	127.451	7.50	5.88	13.94	6.97	4.65	5.67	4.64	3.72
85	1.3	171*	14.00	8.19	26.97	13.49	8.99	6.26	5.81	5.23
68	1.3	203.75*	6.94	3.41	36.78	18.39	12.26	15.95	12.75	10.08
70	1.2	287.8*	37.22	12.93	61.94	30.97	20.65	5.54	5.47	5.37
W [mg/kg]										
85	1.3	178	18.00	10.11	-	-	-	-	-	-
68	1.3	209.95	19.17	9.13	-	-	-	-	-	-
Y (31.8 ± 3.02) [mg/kg]										
4	1.1	10.9	2.90	26.61	-13.83	-6.92	-4.61	6.39	4.99	3.88
84	1.2	12.19	1.90	15.59	-12.98	-6.49	-4.33	8.08	5.49	3.99
72	1.4	12.615	1.36	10.76	-12.70	-6.35	-4.23	9.45	5.79	4.05
54	1.0	24	2.10	8.75	-5.16	-2.58	-1.72	3.01	2.12	1.56
37	1.2	24.135	0.82	3.41	-5.07	-2.54	-1.69	4.45	2.45	1.66
77	1.0	26	1.60	6.15	-3.84	-1.92	-1.28	2.64	1.70	1.21
71	1.1	26.86	8.04	29.93	-3.27	-1.63	-1.09	0.60	0.58	0.54
15	1.3	27.2	2.30	8.46	-3.04	-1.52	-1.01	1.67	1.21	0.90
74	2.0	28.3	2.22	7.84	-2.32	-1.16	-0.77	1.30	0.93	0.69
56	1.3	29	1.20	4.14	-1.85	-0.93	-0.62	1.45	0.86	0.60
62	1.3	29.615	2.53	8.53	-1.45	-0.72	-0.48	0.74	0.55	0.42
69	1.1	30	17.00	56.67	-1.19	-0.60	-0.40	0.11	0.10	0.10
87	1.3	30.67	0.33	1.08	-0.75	-0.37	-0.25	0.73	0.37	0.25
21	2.0	32.4	0.50	1.54	0.40	0.20	0.13	0.38	0.20	0.13
64	1.1	36	3.00	8.33	2.78	1.39	0.93	1.25	0.99	0.77
85	1.3	38.3	3.50	9.14	4.30	2.15	1.43	1.71	1.41	1.13
63	1.2	39.8	5.50	13.82	5.29	2.65	1.76	1.40	1.27	1.12
76	1.3	44.07	2.02	4.58	8.12	4.06	2.71	4.86	3.38	2.47
73	1.0	205.914*	10.22	4.96	115.22	57.61	38.41	16.86	16.34	15.58
70	1.2	292.3*	129.40	44.27	172.38	86.19	57.46	2.01	2.01	2.01
Yb [mg/kg]										
85	1.3	2.2	0.20	9.09	-	-	-	-	-	-
87	1.3	2.696	0.05	1.97	-	-	-	-	-	-
61	5.0	3.51	0.15	4.19	-	-	-	-	-	-
Zn (96.1 ± 7.73) [mg/kg]										
86	1.2	61.18	2.65	4.33	-9.03	-4.52	-3.01	7.45	4.27	2.93
54	1.0	66.6	5.50	8.26	-7.63	-3.81	-2.54	4.39	3.11	2.30

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED *z*- AND *u*-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	<i>z</i> -scores			<i>u</i> -scores		
					<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5
84	1.2	78.73	5.70	7.24	-4.49	-2.25	-1.50	2.52	1.81	1.34
72	1.4	83.474	1.40	1.68	-3.27	-1.63	-1.09	3.07	1.61	1.08
69	1.1	89	6.00	6.74	-1.84	-0.92	-0.61	0.99	0.73	0.54
74	2.0	95.6	2.55	2.67	-0.13	-0.06	-0.04	0.11	0.06	0.04
58	1.0	95.8	7.60	7.93	-0.08	-0.04	-0.03	0.04	0.03	0.02
37	1.2	95.931	0.46	0.47	-0.04	-0.02	-0.01	0.04	0.02	0.01
21	2.0	96.1	1.20	1.25	0.00	0.00	0.00	0.00	0.00	0.00
15	1.3	96.5	7.70	7.98	0.10	0.05	0.03	0.05	0.04	0.03
57	1.4	97.4	2.10	2.16	0.34	0.17	0.11	0.30	0.16	0.11
64	1.1	98	7.00	7.14	0.49	0.25	0.16	0.24	0.18	0.14
55	5.0	98.18	25.62	26.09	0.54	0.27	0.18	0.08	0.08	0.07
53	2.0	100	10.00	10.00	1.01	0.50	0.34	0.36	0.31	0.25
56	1.3	100.5	5.00	4.98	1.14	0.57	0.38	0.70	0.48	0.35
82	1.2	102.2	2.90	2.84	1.58	0.79	0.53	1.26	0.74	0.51
85	1.3	103	11.00	10.68	1.78	0.89	0.59	0.59	0.51	0.43
78	1.1	104	1.00	0.96	2.04	1.02	0.68	1.98	1.01	0.68
24	1.1	106.902	12.22	11.43	2.79	1.40	0.93	0.84	0.75	0.64
63	1.2	107	9.00	8.41	2.82	1.41	0.94	1.11	0.92	0.74
88	1.0	108	9.69	8.97	3.08	1.54	1.03	1.14	0.96	0.79
79	1.3	115	2.12	1.84	4.89	2.44	1.63	4.29	2.36	1.60
87	1.3	122.864	0.14	0.11	6.92	3.46	2.31	6.92	3.46	2.31
62	1.3	123.564	4.42	3.58	7.10	3.55	2.37	4.68	3.08	2.21
77	1.0	124	6.30	5.08	7.22	3.61	2.41	3.77	2.80	2.11
76	1.3	137.43	15.18	11.05	10.69	5.34	3.56	2.64	2.43	2.16
59	1.2	160	11.00	6.88	16.53	8.26	5.51	5.48	4.75	4.00
70	1.2	161.6*	65.04	40.25	16.94	8.47	5.65	1.01	1.00	0.99
71	1.1	169.94*	63.29	37.24	19.10	9.55	6.37	1.16	1.16	1.15
68	1.3	255.75*	5.13	2.01	41.29	20.65	13.76	24.85	17.20	12.59
73	1.0	513.401*	18.02	3.51	107.93	53.96	35.98	22.64	21.28	19.47
Zr (302 ± 20.45) [mg/kg]										
4	1.1	26.2*	1.30	4.96	-26.97	-13.48	-8.99	26.75	13.46	8.98
77	1.0	169	9.30	5.50	-13.00	-6.50	-4.33	9.62	5.92	4.15
62	1.3	234.357	10.57	4.51	-6.61	-3.31	-2.20	4.60	2.94	2.08
54	1.0	262	5.10	1.95	-3.91	-1.96	-1.30	3.50	1.90	1.29
15	1.3	281	18.60	6.62	-2.05	-1.03	-0.68	0.99	0.76	0.59
24	1.1	293.374	42.36	14.44	-0.84	-0.42	-0.28	0.20	0.18	0.16
74	2.0	295.4	3.03	1.02	-0.65	-0.32	-0.22	0.62	0.32	0.21
69	1.1	305	18.00	5.90	0.29	0.15	0.10	0.14	0.11	0.08
64	1.1	307	12.00	3.91	0.49	0.24	0.16	0.32	0.21	0.15
56	1.3	310.3	15.00	4.83	0.81	0.41	0.27	0.46	0.33	0.24
63	1.2	316	25.00	7.91	1.37	0.68	0.46	0.52	0.43	0.35
55	1.2	316.865	3.05	0.96	1.45	0.73	0.48	1.39	0.72	0.48
21	2.0	317	5.60	1.77	1.47	0.73	0.49	1.29	0.71	0.48
71	1.1	332.93	96.97	29.13	3.02	1.51	1.01	0.32	0.31	0.30

TABLE 3 (cont.). SUMMARY OF THE REPORTED RESULTS AND THE CALCULATED z- AND u-SCORES

Laboratory code	Technique code	Analyte concentration	Standard dev.	Relative std. dev., [%]	z-scores			u-scores		
					$k = 0.5$	$k = 1.0$	$k = 1.5$	$k = 0.5$	$k = 1.0$	$k = 1.5$
87	1.3	333.215	1.32	0.40	3.05	1.53	1.02	3.03	1.52	1.02
82	1.2	341.1	8.50	2.49	3.82	1.91	1.27	2.94	1.77	1.23
76	1.3	381.29	28.40	7.45	7.75	3.88	2.58	2.63	2.27	1.90
59	1.2	395	42.00	10.63	9.09	4.55	3.03	2.15	1.99	1.79
68	1.3	416.38	1.98	0.48	11.18	5.59	3.73	10.98	5.57	3.72
85	1.3	433	43.00	9.93	12.81	6.40	4.27	2.96	2.75	2.48
70	1.2	1295.2*	400.00	30.88	97.11	48.56	32.37	2.48	2.48	2.48
73	1.0	1940.166*	14.45	0.74	160.17	80.09	53.39	92.55	65.42	48.30

TABLE 4. THE COMBINED *z*-SCORES FOR THE PARTICIPATING LABORATORIES

Lab Code	Number of analytes	Rescaled sum of scores (RSZ)			Sum of squared scores (SSZ)			Critical value
		<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	<i>k</i> = 0.5	<i>k</i> = 1.0	<i>k</i> = 1.5	
4	11	-55.39	-27.69	-18.46	4055	1014	451	21.92
15	18	-5.08	-2.54	-1.69	138.98	34.75	15.44	31.53
21	27	.63	.32	.21	106.92	26.73	11.88	43.19
24	6	.43	.21	.14	42.29	10.57	4.70	14.45
37	28	-5.35	-2.68	-1.78	1039	260	115.41	44.46
53	14	-14.94	-7.47	-4.98	625	156	69.43	26.12
54	14	-20.51	-10.25	-6.84	1136	284	126.18	26.12
55	29	14.71	7.36	4.90	2199	550	244	45.72
56	20	2.37	1.19	.79	231	57.64	25.62	34.17
57	13	-1.85	-.92	-.62	1900	475	211	24.74
58	17	89.70	44.85	29.90	146113	36528	16235	30.19
59	9	25.27	12.64	8.42	1098	275	122.05	19.02
61	14	9.77	4.88	3.26	137.68	34.42	15.30	26.12
62	15	54.95	27.48	18.32	63688	15922	7076	27.49
63	24	41.12	20.56	13.71	43115	10779	4791	39.36
64	21	15.13	7.57	5.04	4377	1094	486	35.48
68	25	425	213	141.68	487480	121870	54164	40.65
69	29	24.98	12.49	8.33	7407	1852	823	45.72
70	18	297	148.74	99.16	245689	61422	27299	31.53
71	14	11.40	5.70	3.80	840	210	93.33	26.12
72	17	-12.07	-6.04	-4.02	1093	273	121.42	30.19
73	15	738	369	246	733083	183271	81454	27.49
74	28	-7.41	-3.71	-2.47	161	40.35	17.93	44.46
76	26	101.09	50.54	33.70	80990	20247	8999	41.92
77	20	-15.93	-7.97	-5.31	1934	483	215	34.17
78	10	-13.82	-6.91	-4.61	956	239	106.18	20.48
79	23	5.37	2.68	1.79	480	120.12	53.38	38.08
82	12	63.86	31.93	21.29	43858	10964	4873	23.34
84	17	-28.09	-14.04	-9.36	8013	2003	890	30.19
85	32	74.56	37.28	24.85	82512	20628	9168	49.48
86	12	15.29	7.65	5.10	1008	252	111.98	23.34
87	36	21.63	10.82	7.21	6821	1705	758	54.44
88	15	5.83	2.92	1.94	773	193	85.93	27.49

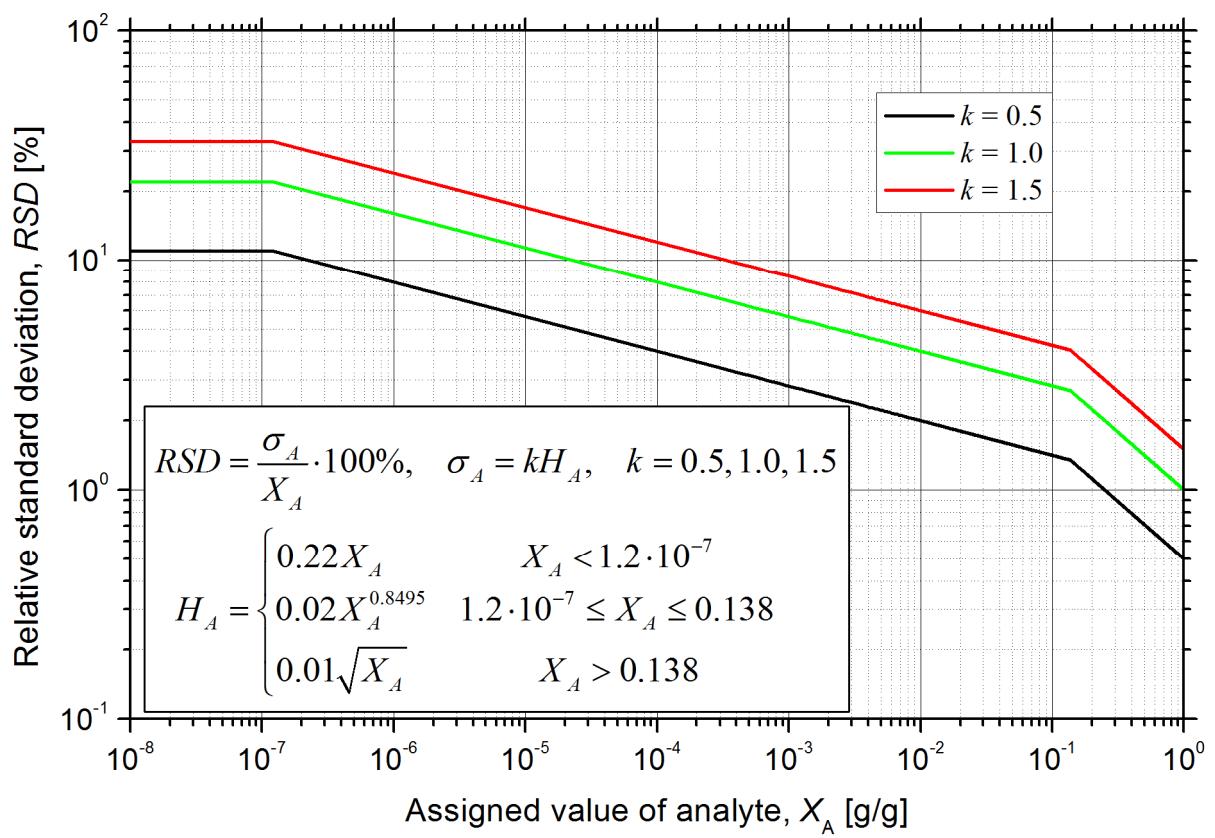


FIG. 1. Relative value of the target standard deviation,  $RSD$ , as a function of the assigned mass fraction of the analyte,  $X_A$ , calculated by using a modified Horowitz function, Eqn. (1).

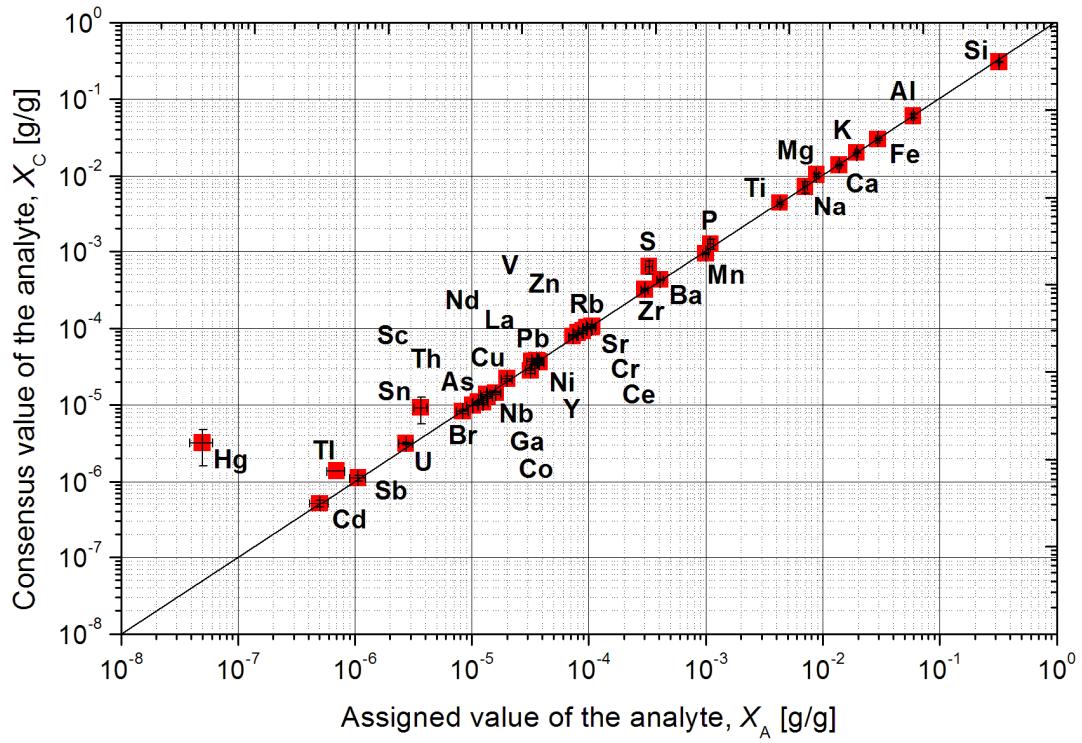


FIG. 2. Correlation between assigned,  $X_A$ , and consensus values of analytes,  $X_C$ <sup>1</sup>.

---

<sup>1</sup> Solid red squares correspond to the elements the assigned values of which were known with high degree of accuracy. The uncertainties of the assigned values were calculated according to Eqn. (2) with  $k = 1$ . The uncertainties of the consensus values were calculated according to Eqn. (20), except for the results reported by a single laboratory, in such a case the laboratory estimate of the uncertainty was shown in the plot.

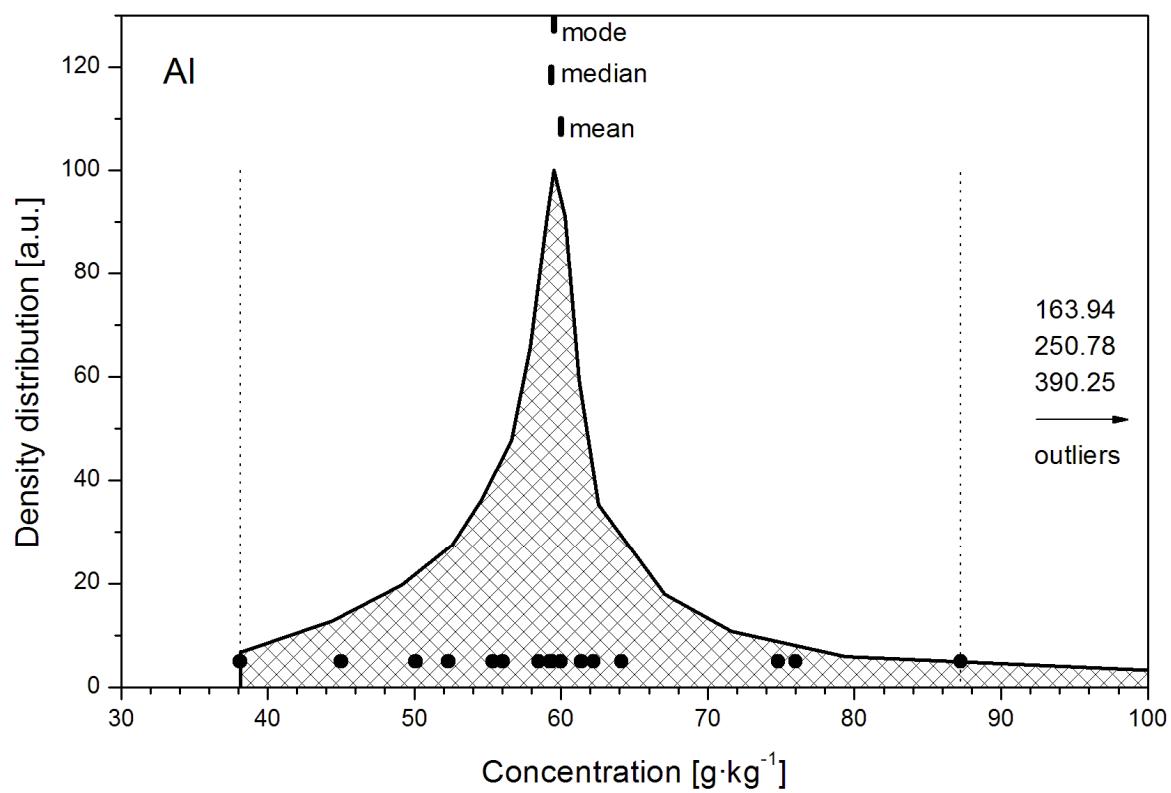


FIG. 3. The density distribution function for the analyte Al.

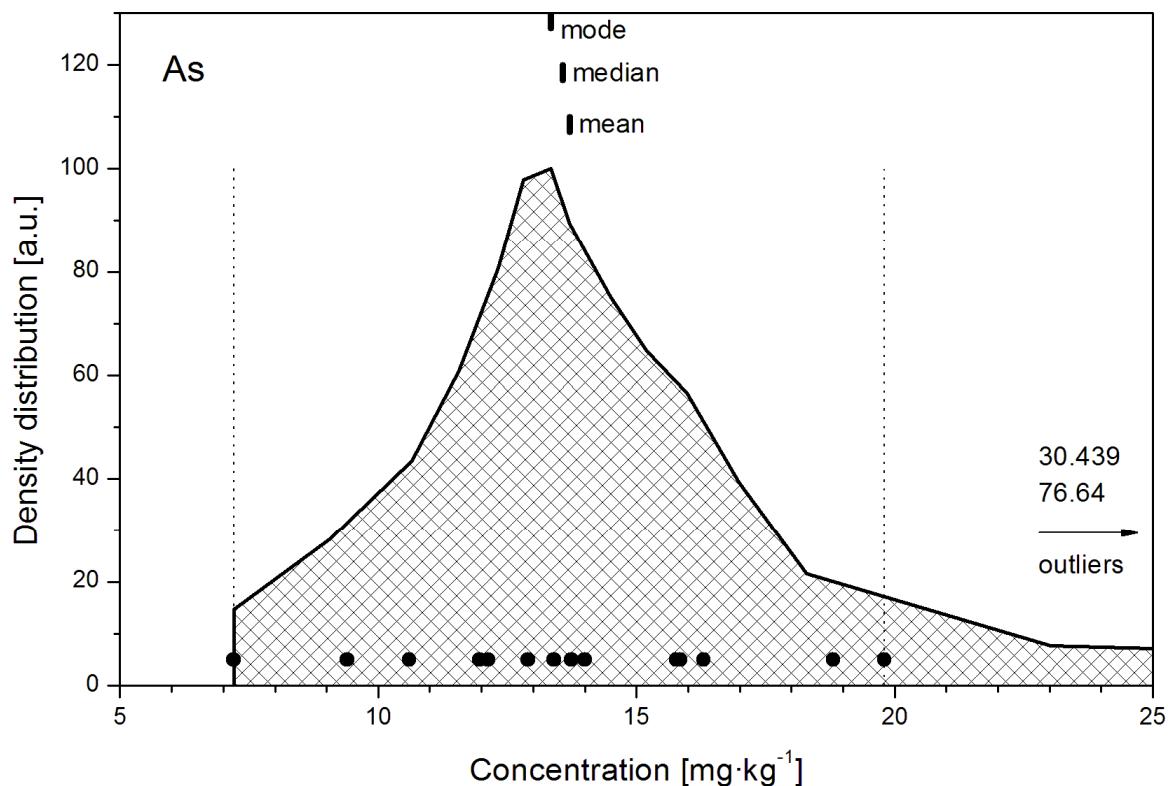


FIG. 4. The density distribution function for the analyte As.

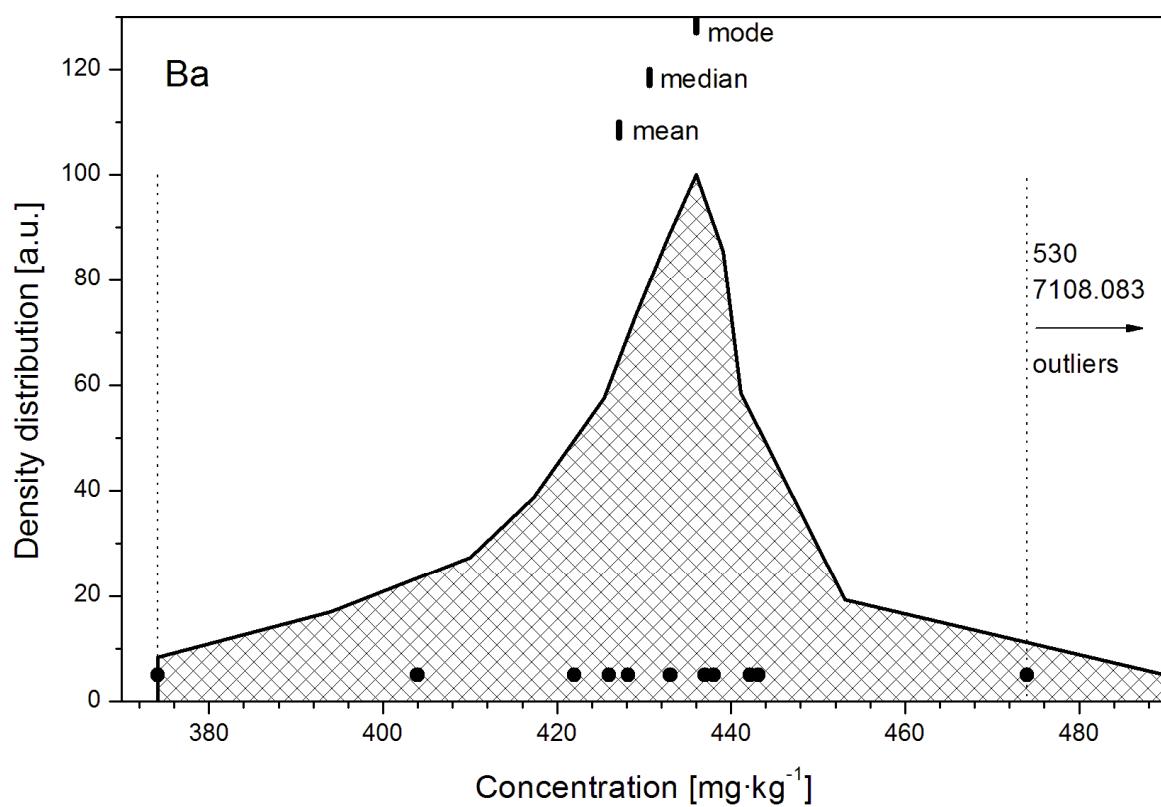


FIG. 5. The density distribution function for the analyte Ba.

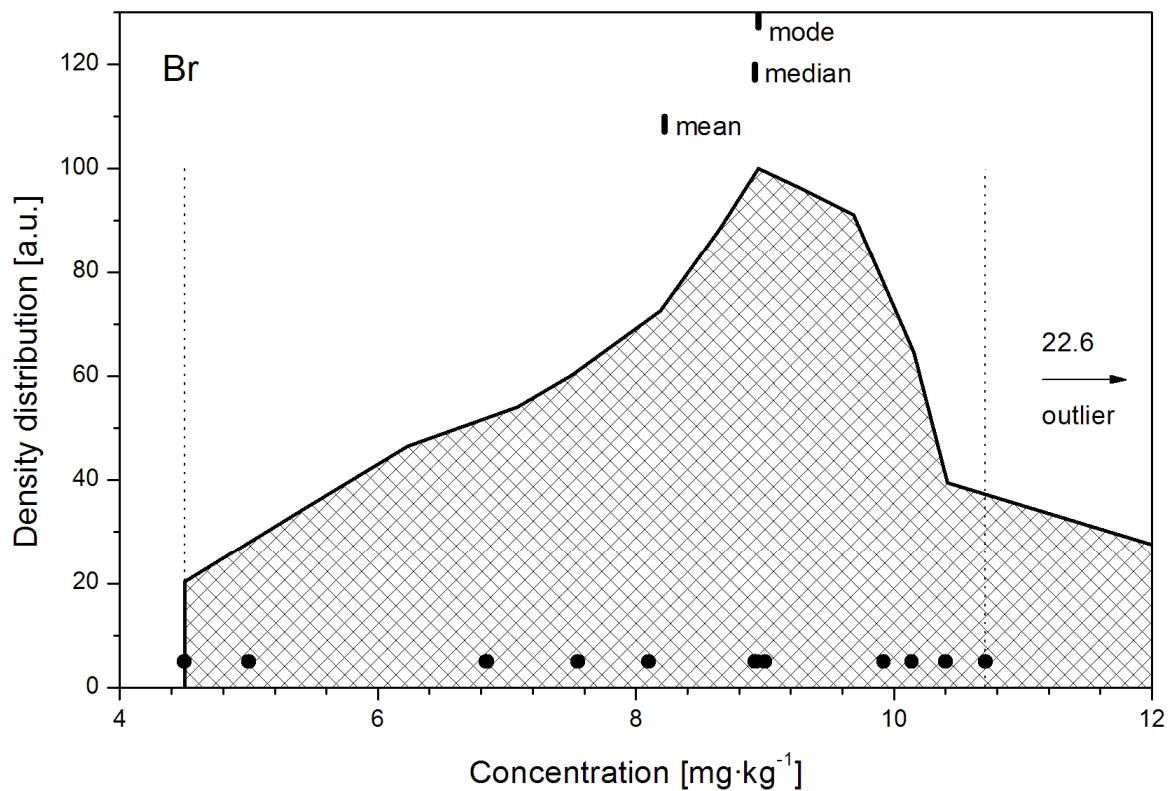


FIG. 6. The density distribution function for the analyte Br.

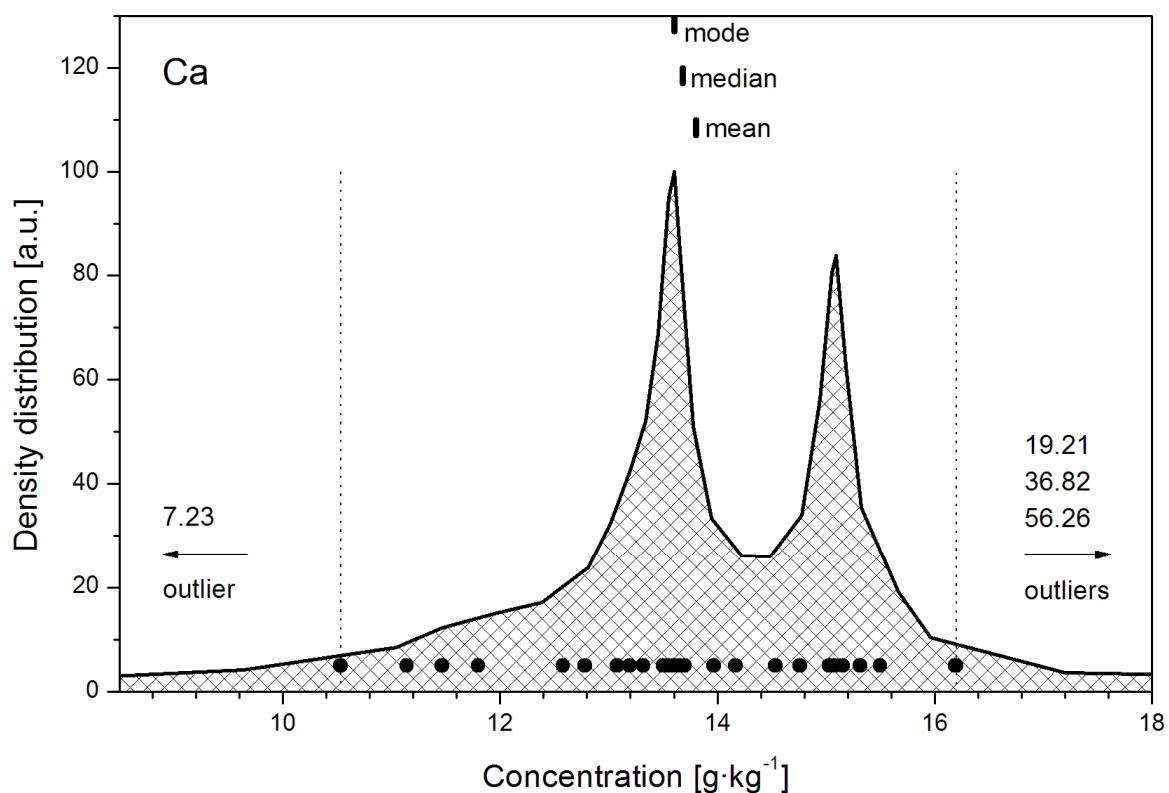


FIG. 7. The density distribution function for the analyte Ca.

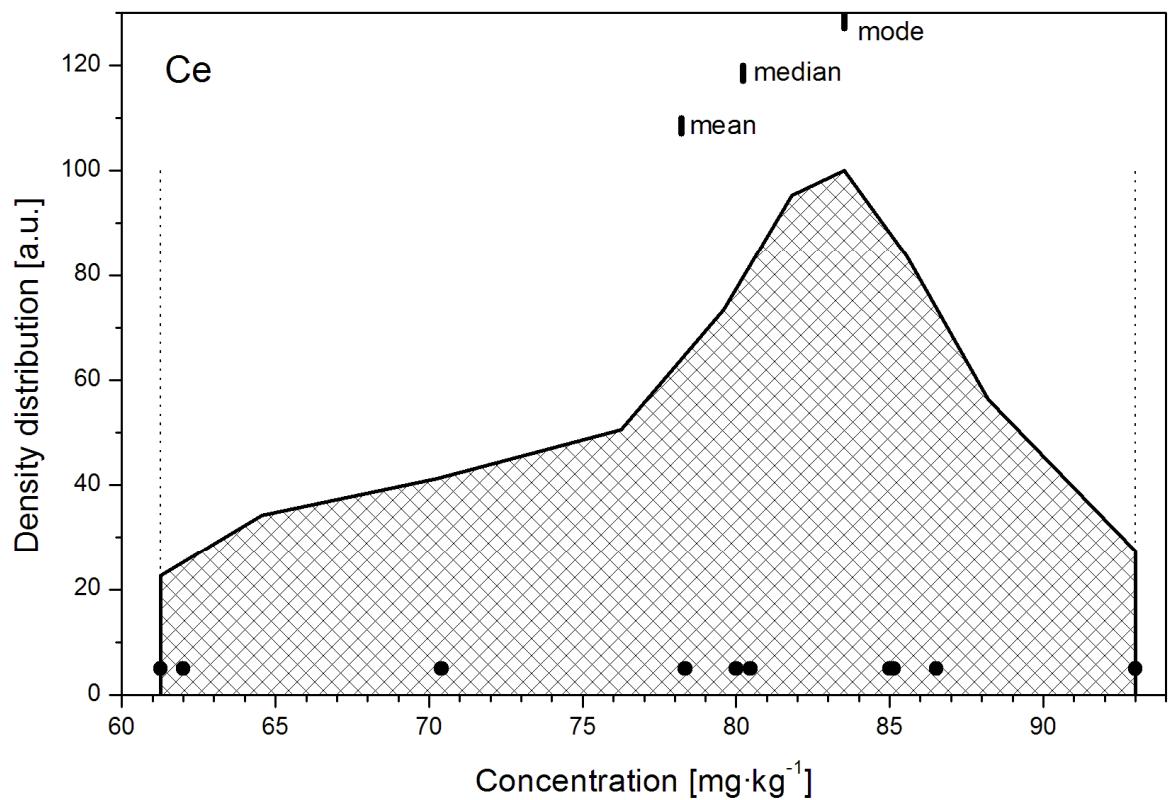


FIG. 8. The density distribution function for the analyte Ce.

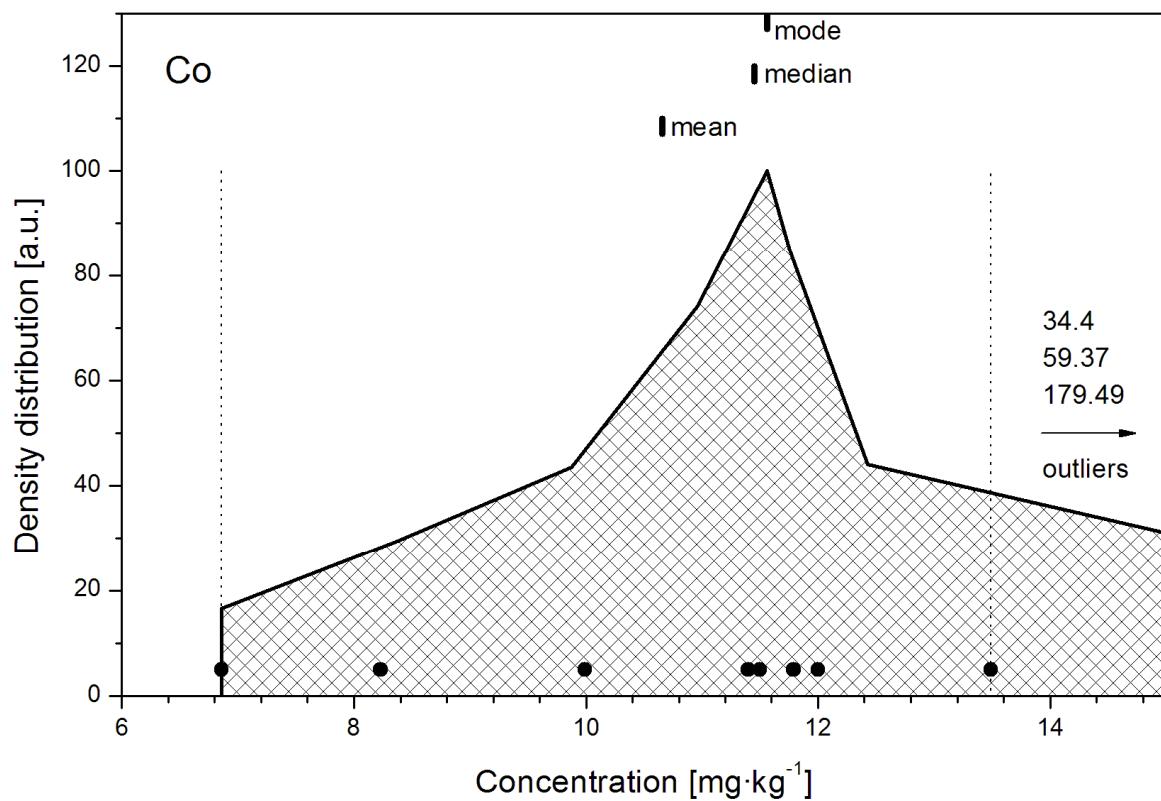


FIG. 9. The density distribution function for the analyte Co.

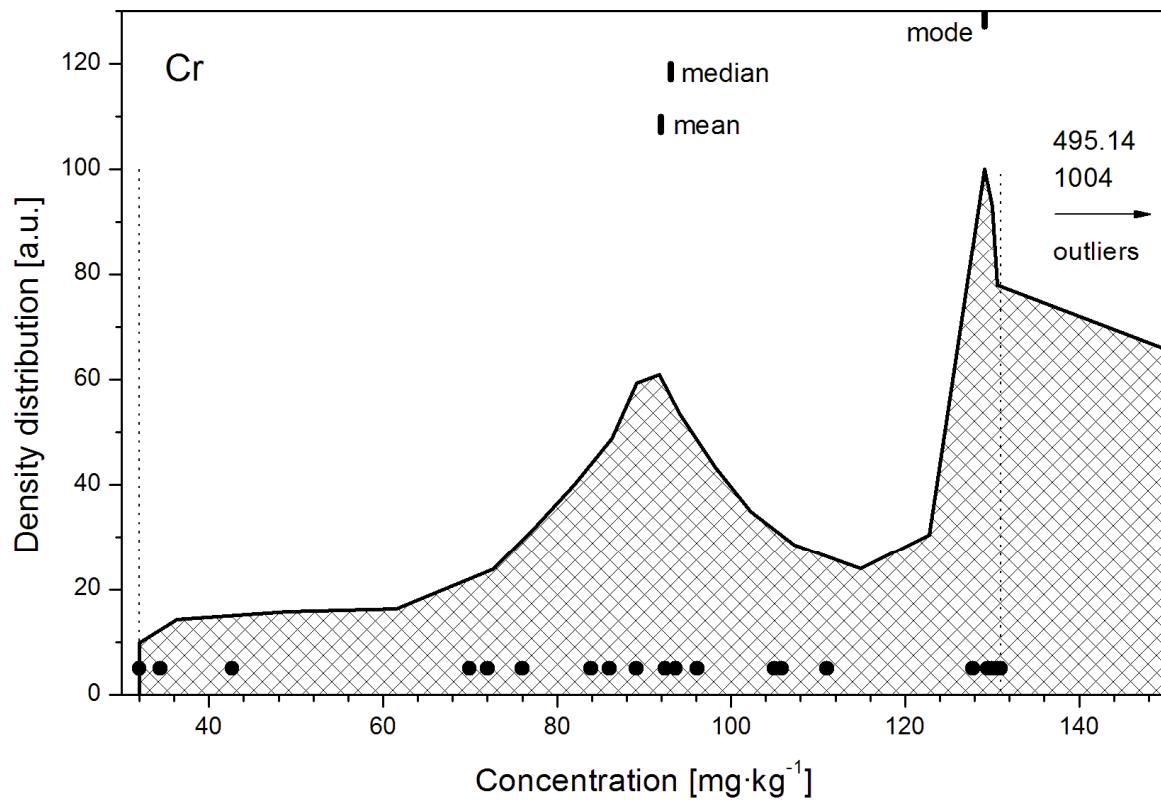


FIG. 10. The density distribution function for the analyte Cr.

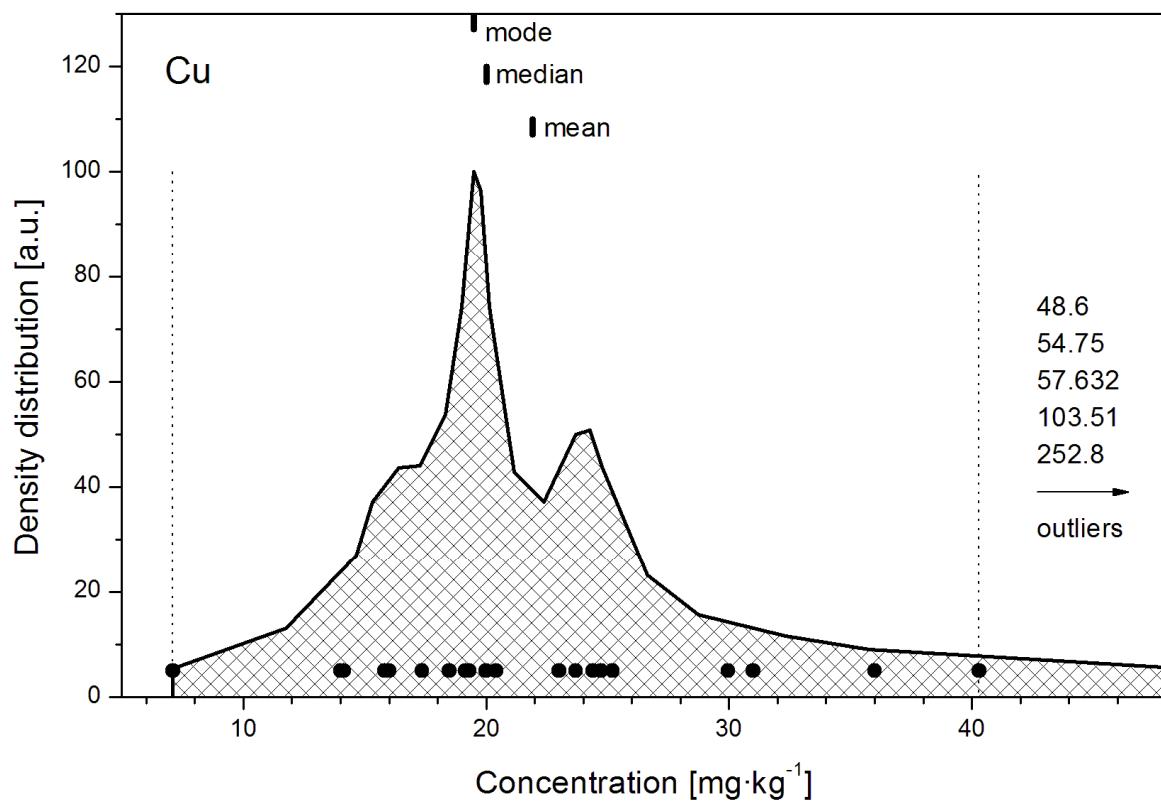


FIG. 11. The density distribution function for the analyte Cu.

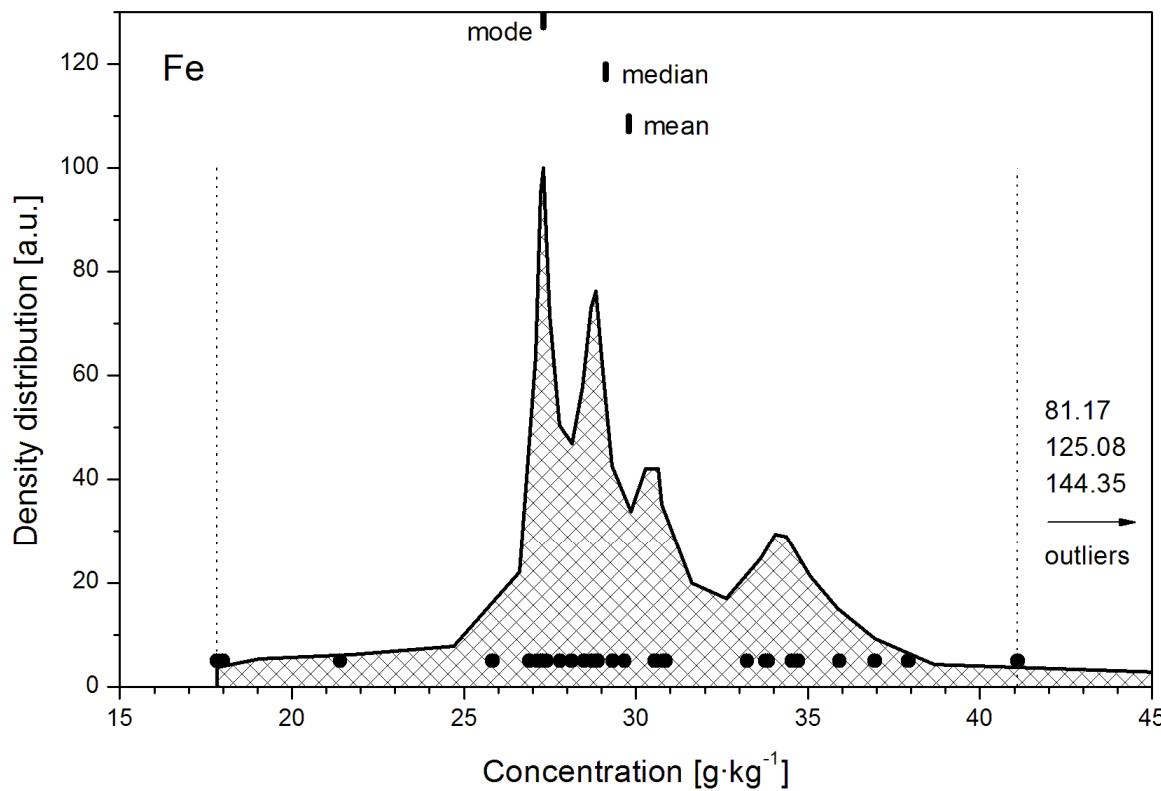


FIG. 12. The density distribution function for the analyte Fe.

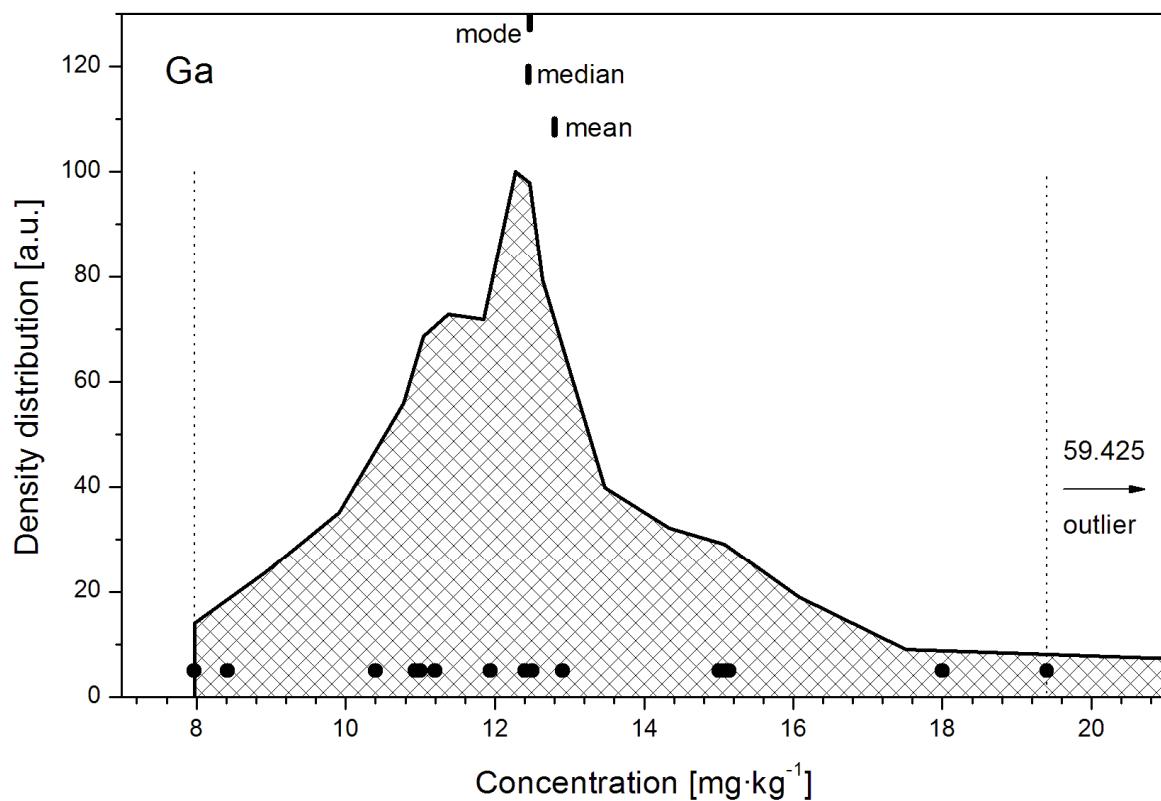


FIG. 13. The density distribution function for the analyte Ga.

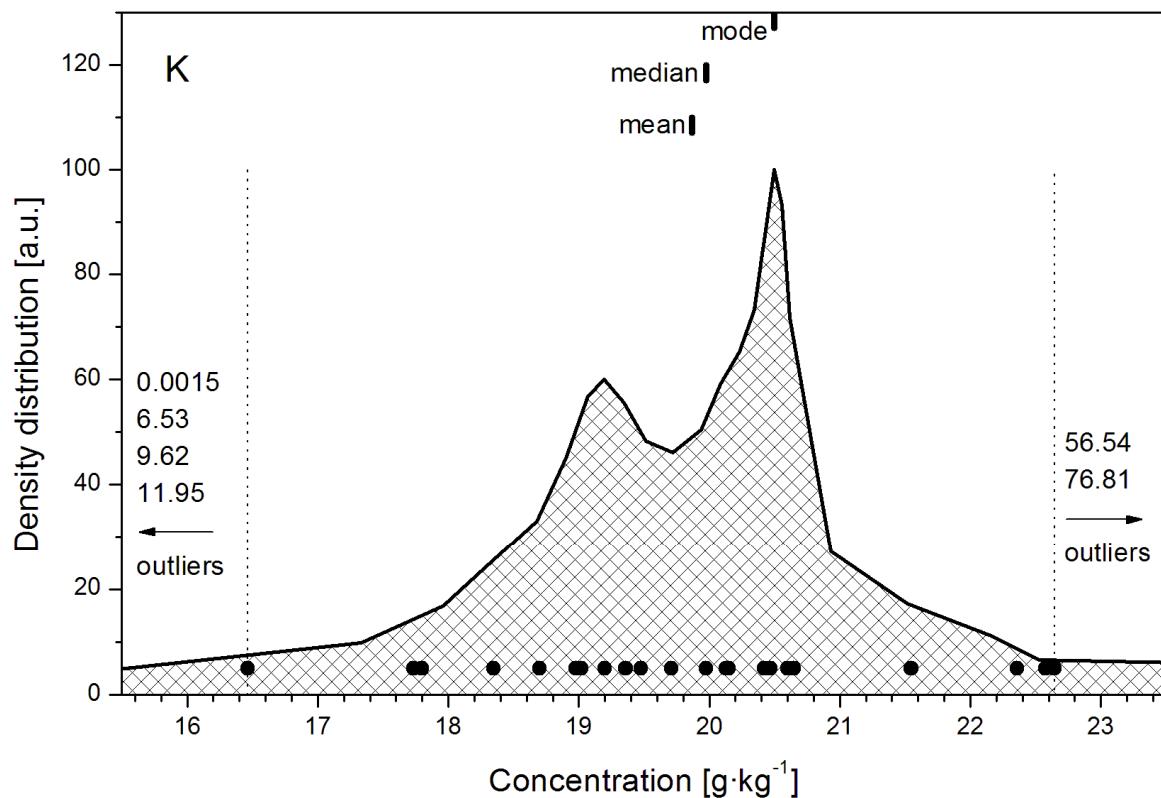


FIG. 14. The density distribution function for the analyte K.

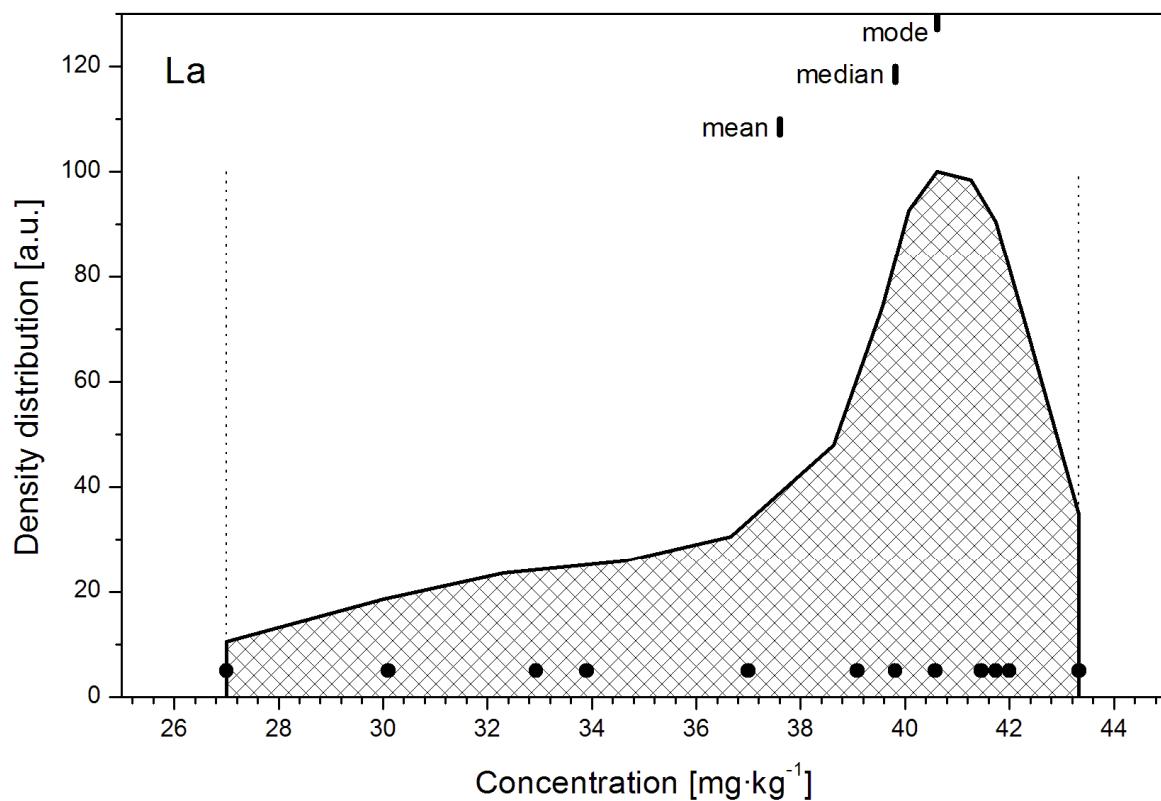


FIG. 15. The density distribution function for the analyte La.

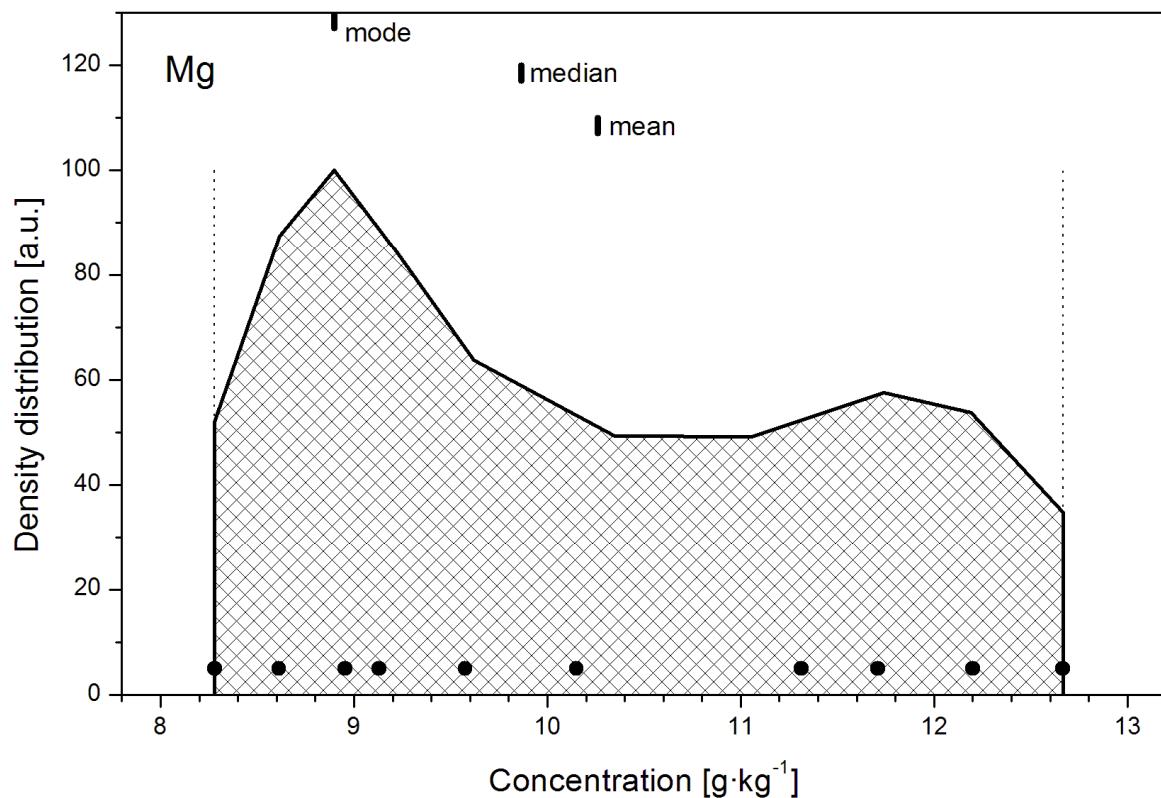


FIG. 16. The density distribution function for the analyte Mg.

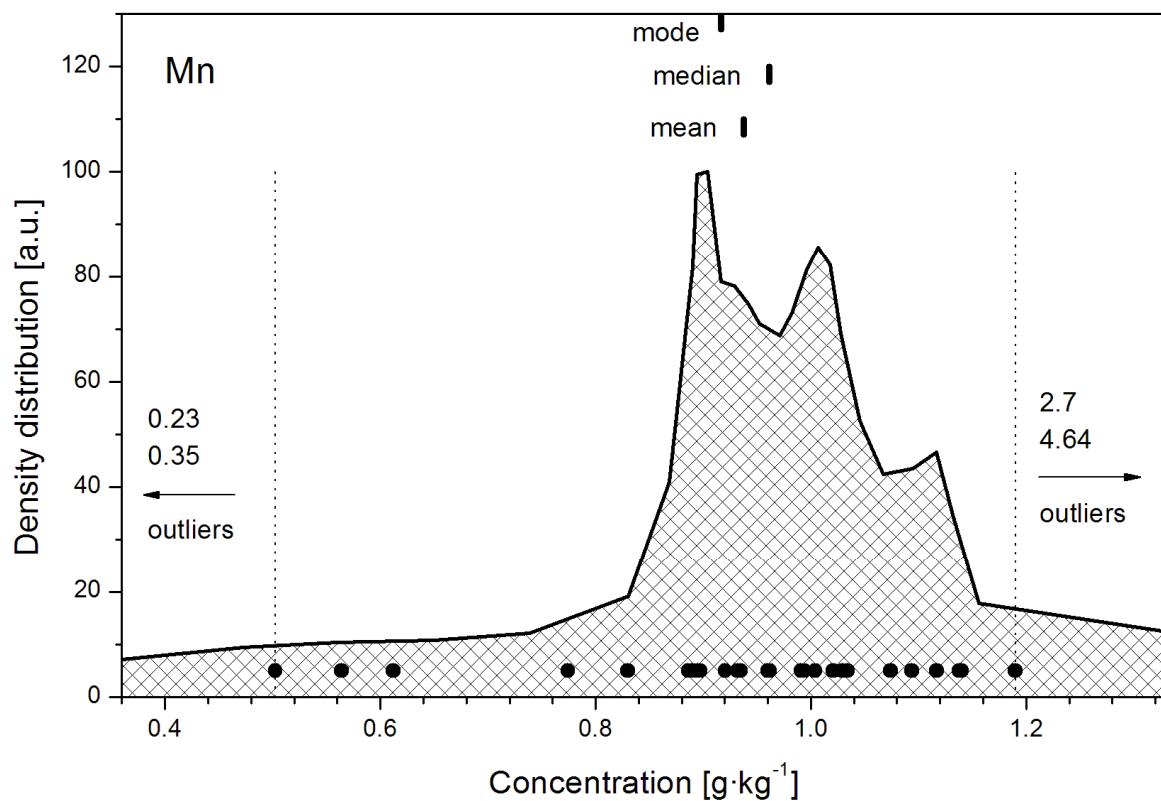


FIG. 17. The density distribution function for the analyte Mn.

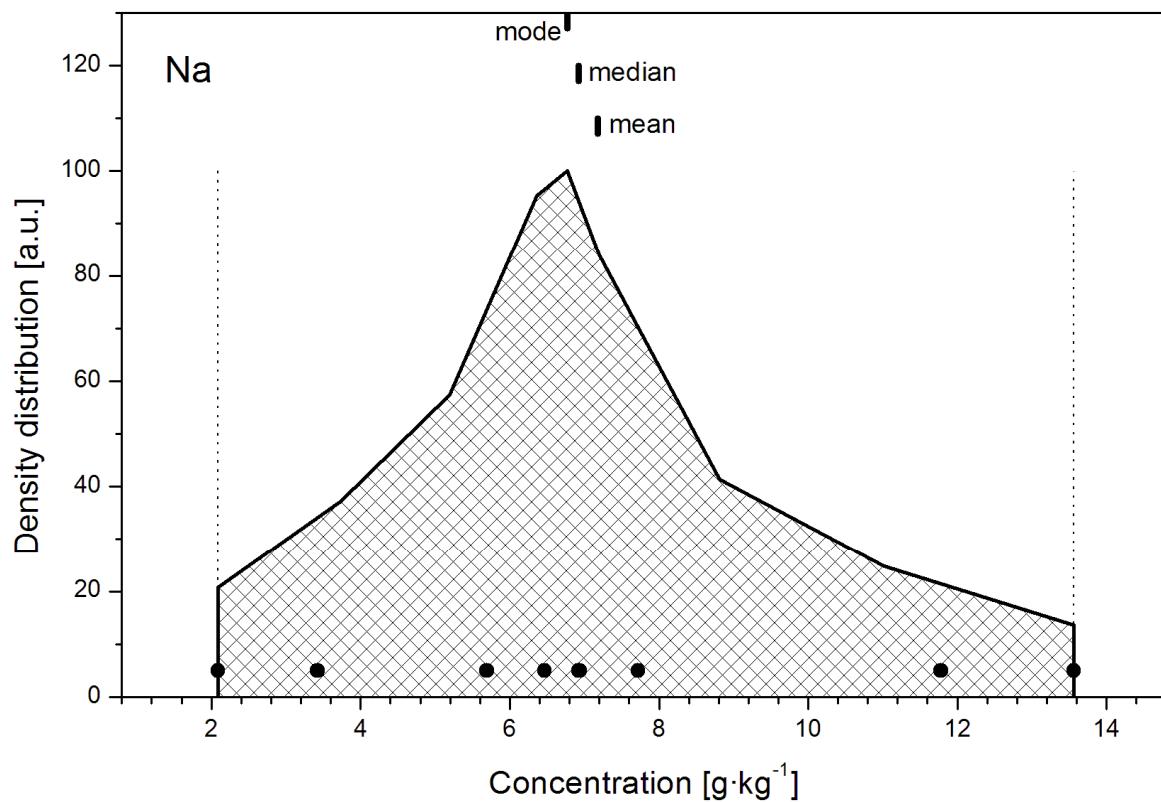


FIG. 18. The density distribution function for the analyte Na.

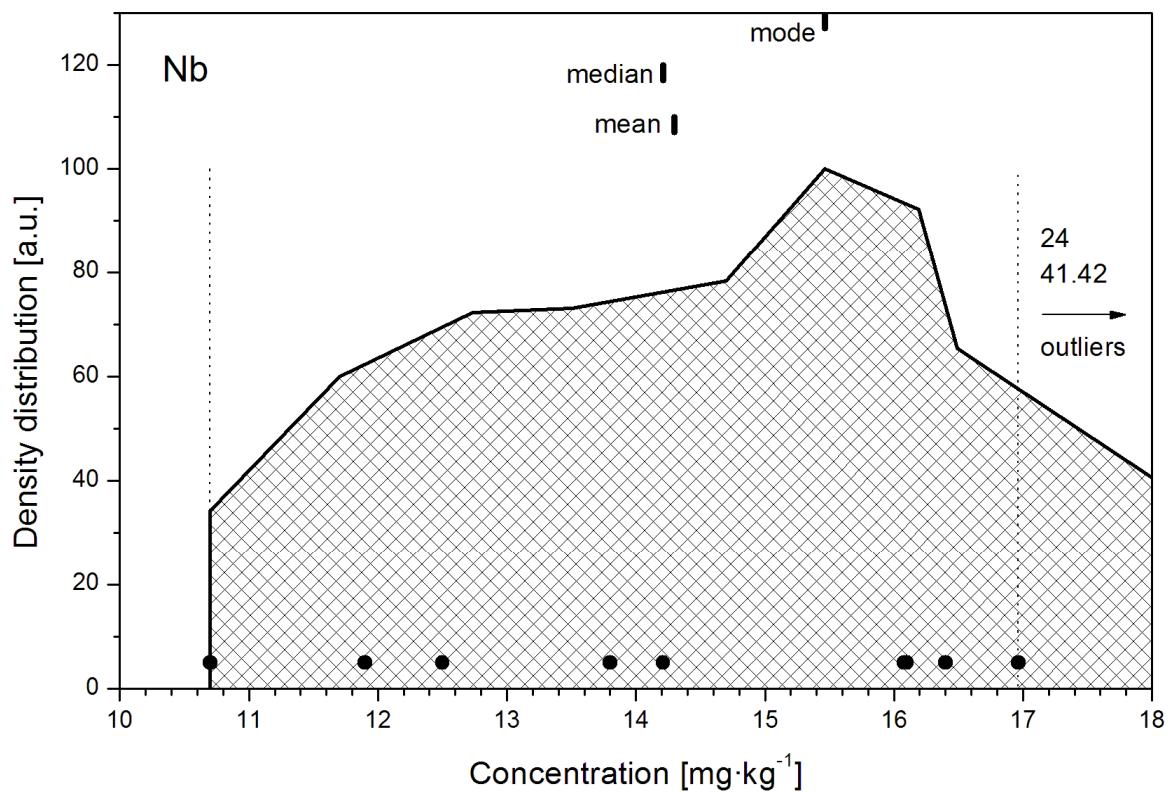


FIG. 19. The density distribution function for the analyte Nb.

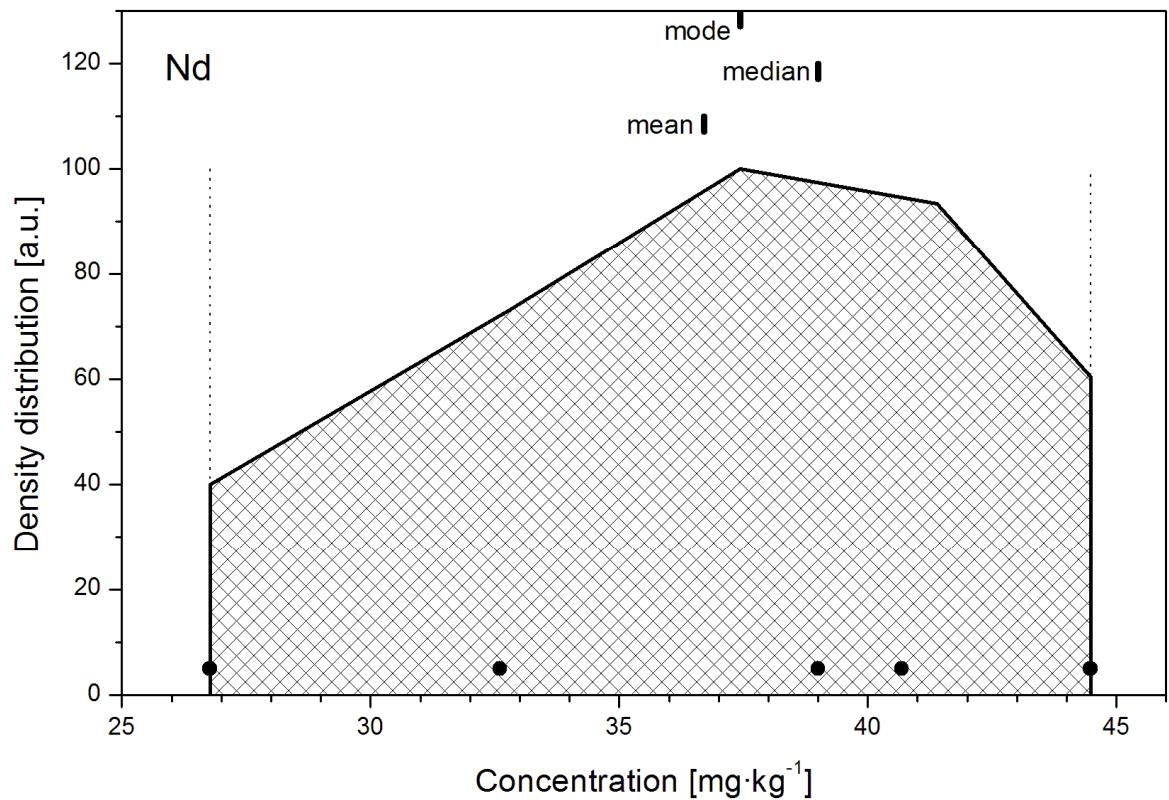


FIG. 20. The density distribution function for the analyte Nd.

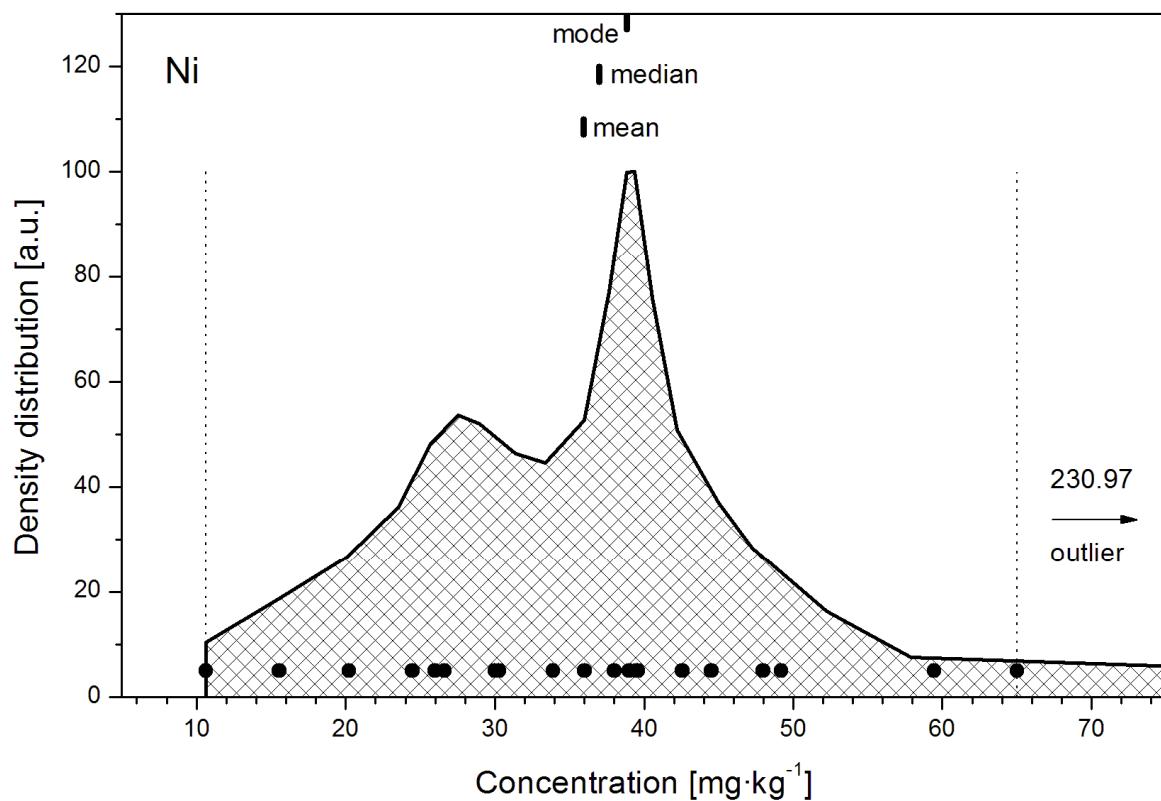


FIG. 21. The density distribution function for the analyte Ni.

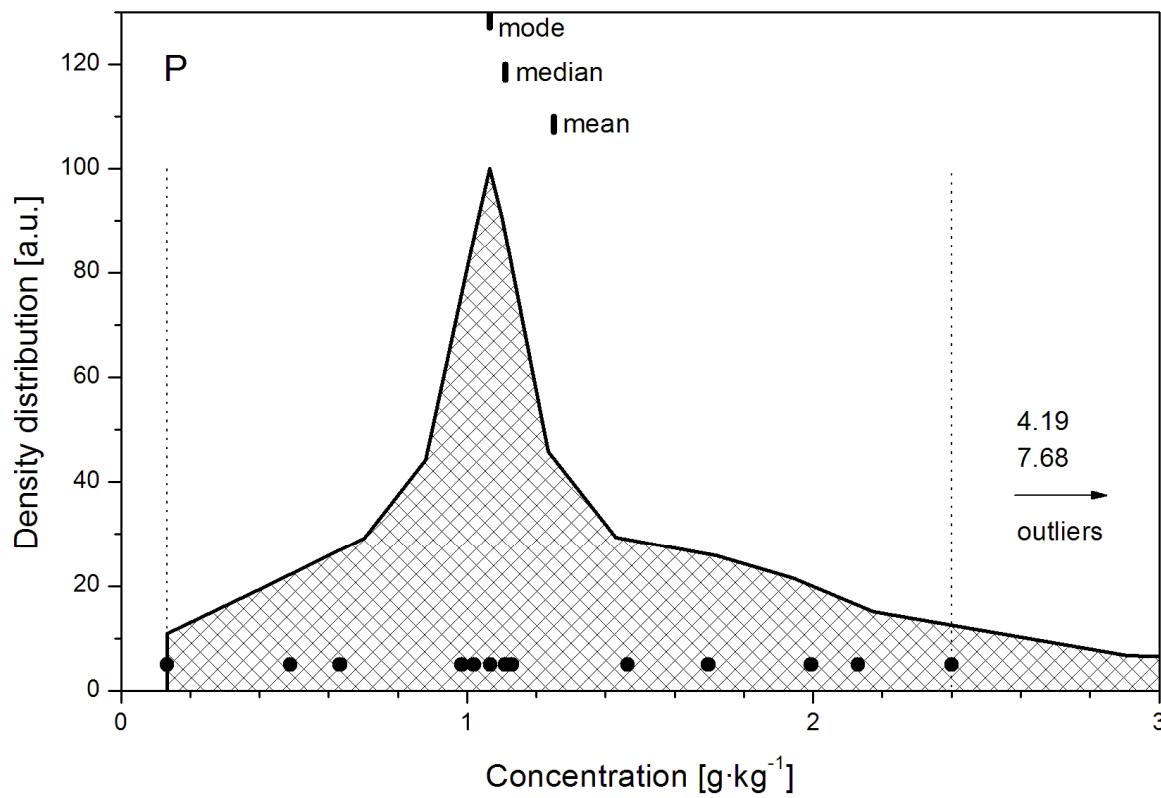


FIG. 22. The density distribution function for the analyte P.

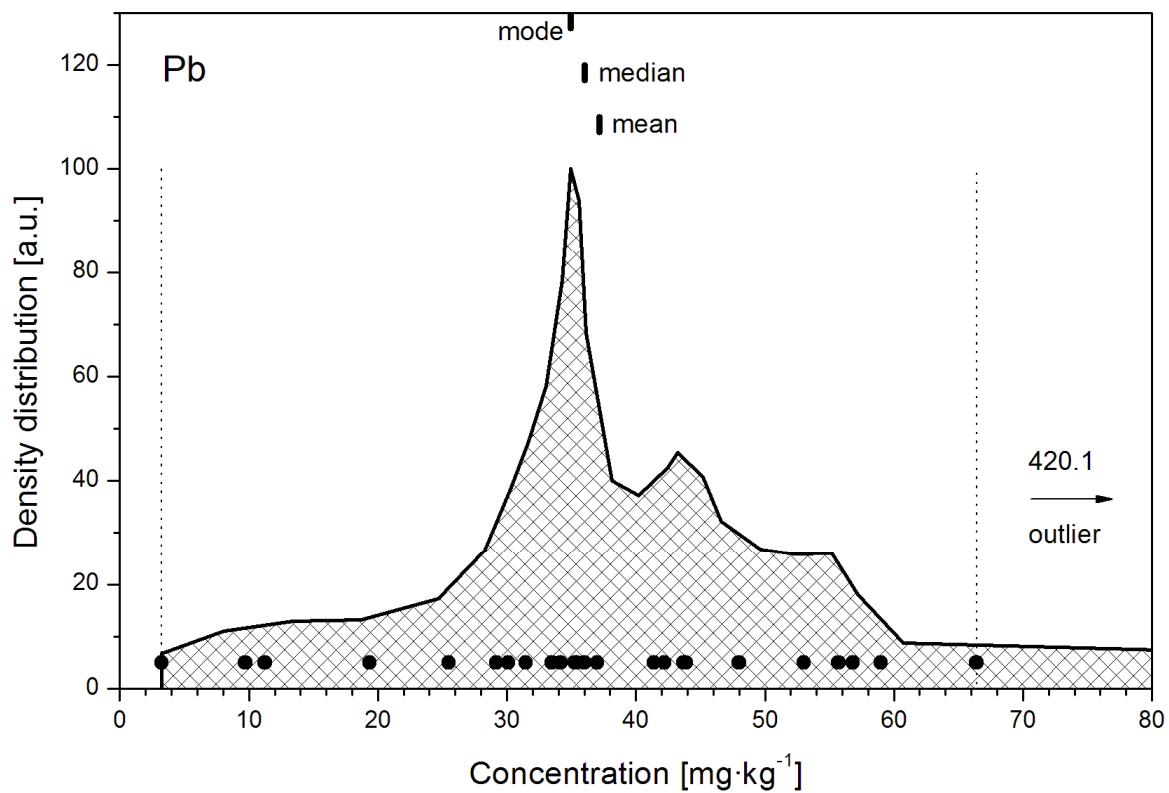


FIG. 23. The density distribution function for the analyte Pb.

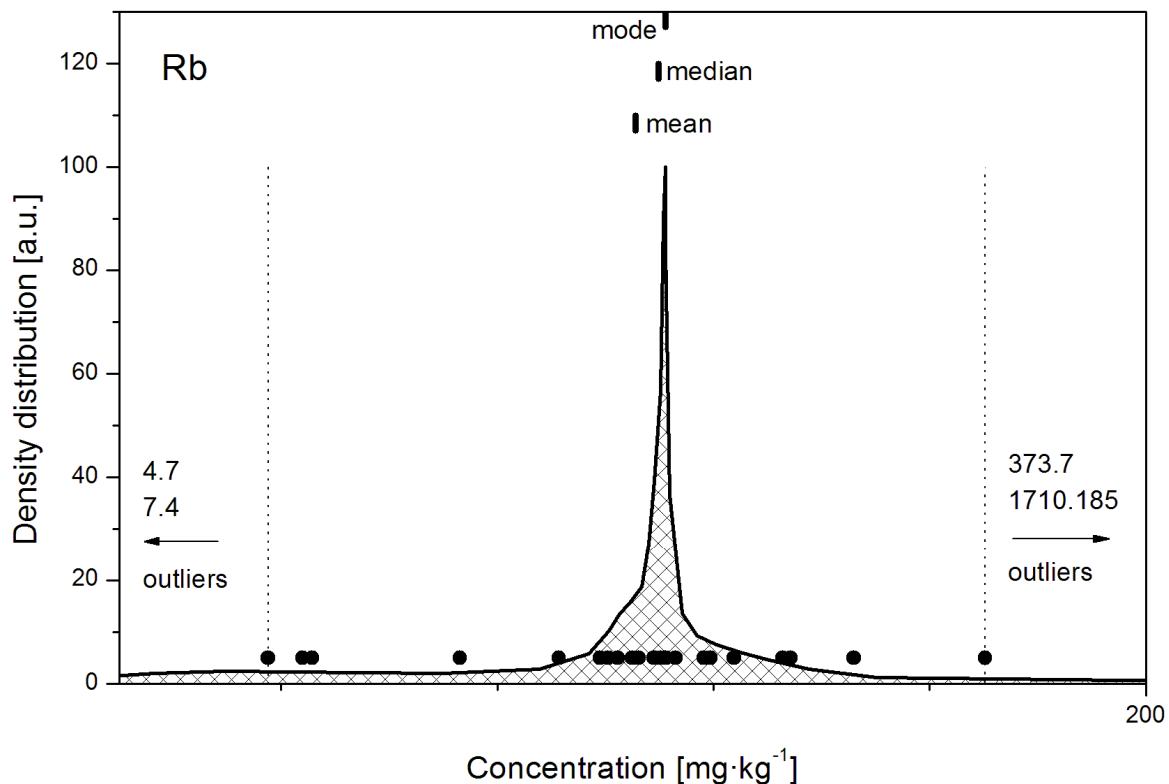


FIG. 24. The density distribution function for the analyte Rb.

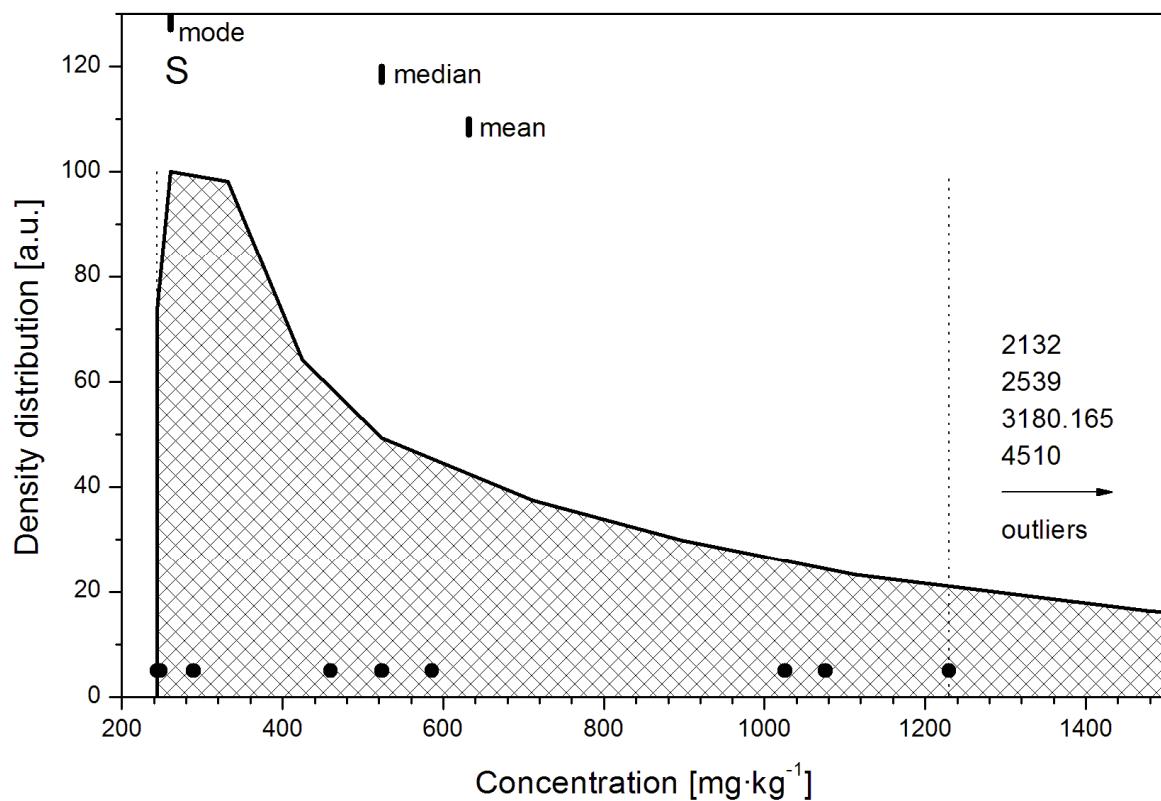


FIG. 25. The density distribution function for the analyte S.

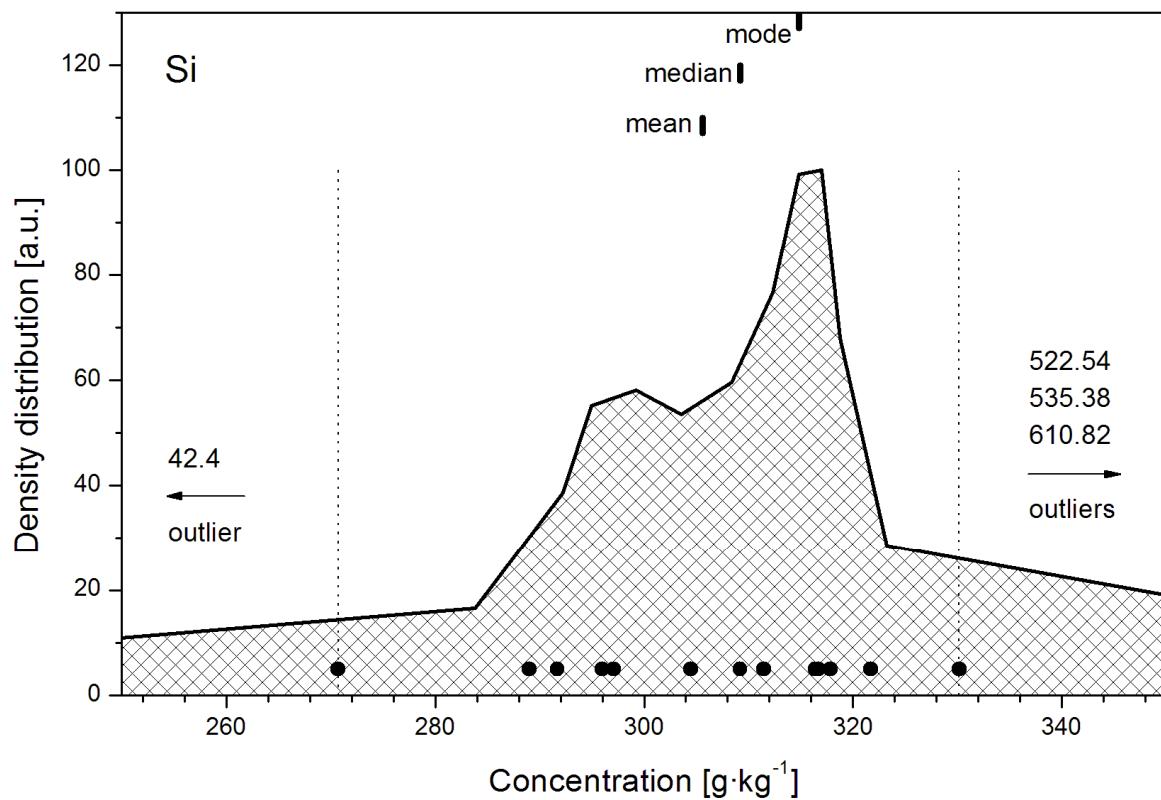


FIG. 26. The density distribution function for the analyte Si.

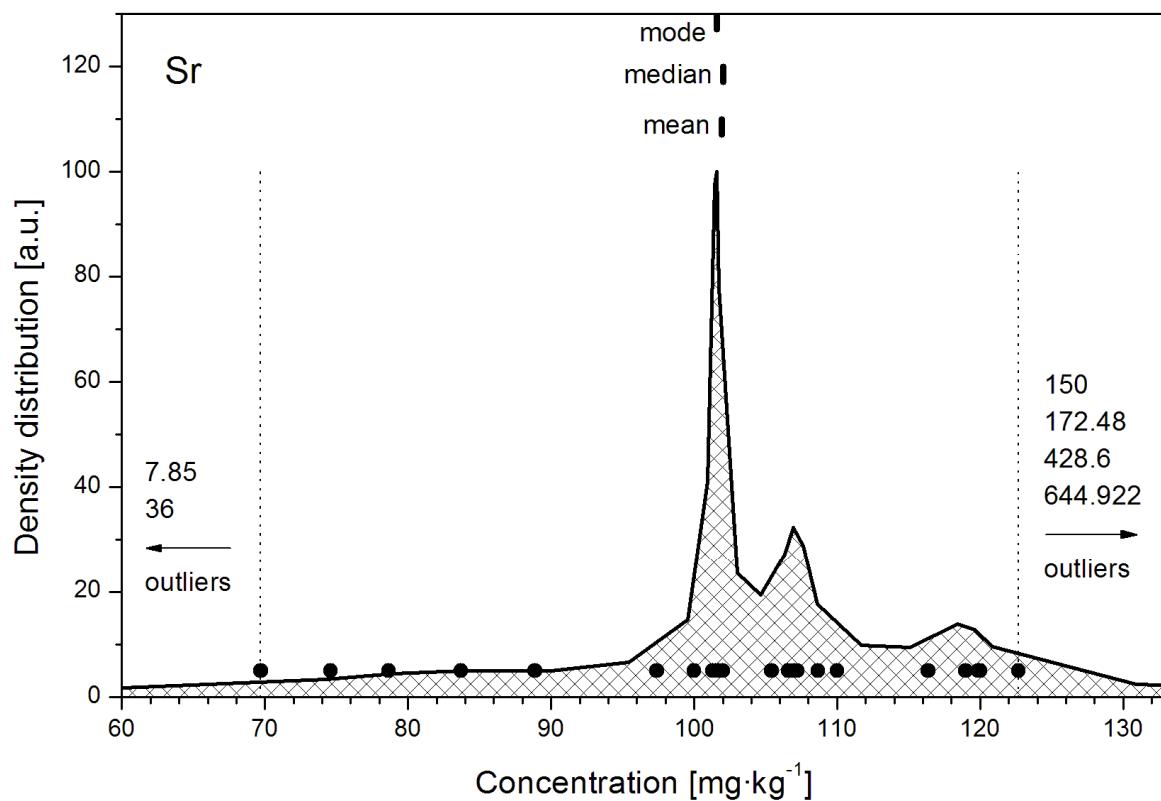


FIG. 27. The density distribution function for the analyte Sr.

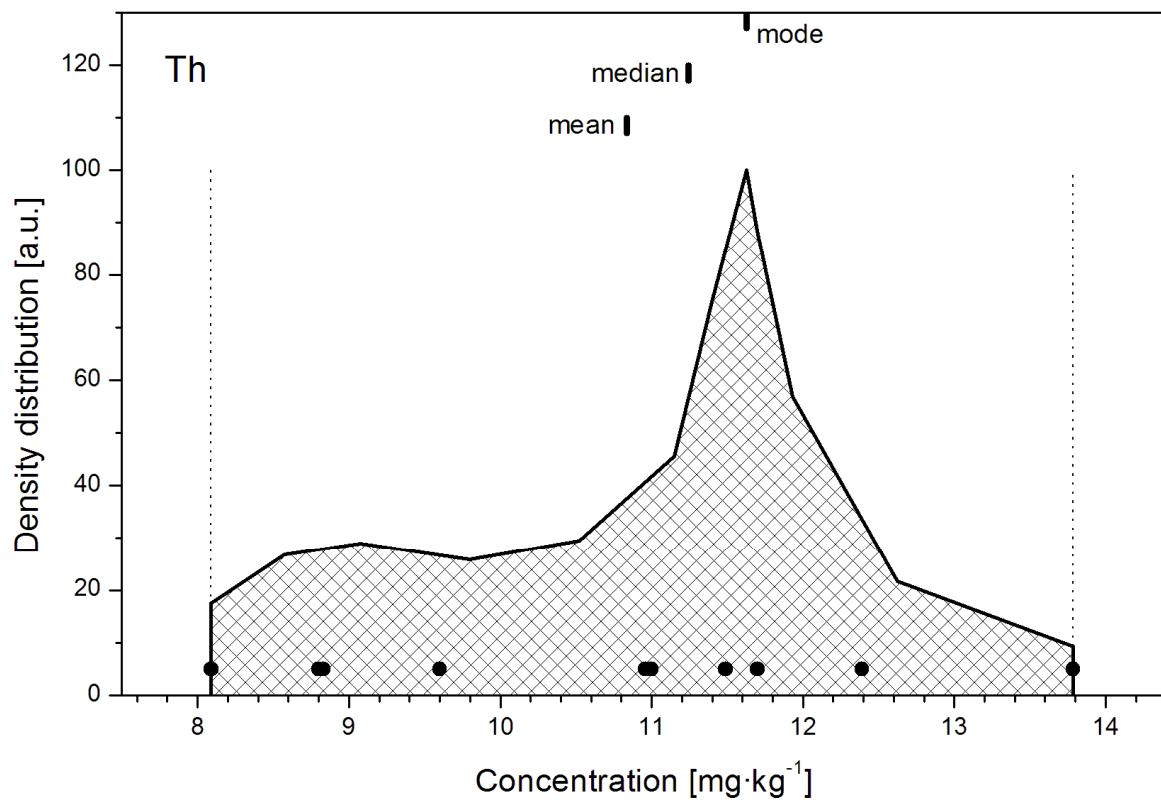


FIG. 28. The density distribution function for the analyte Th.

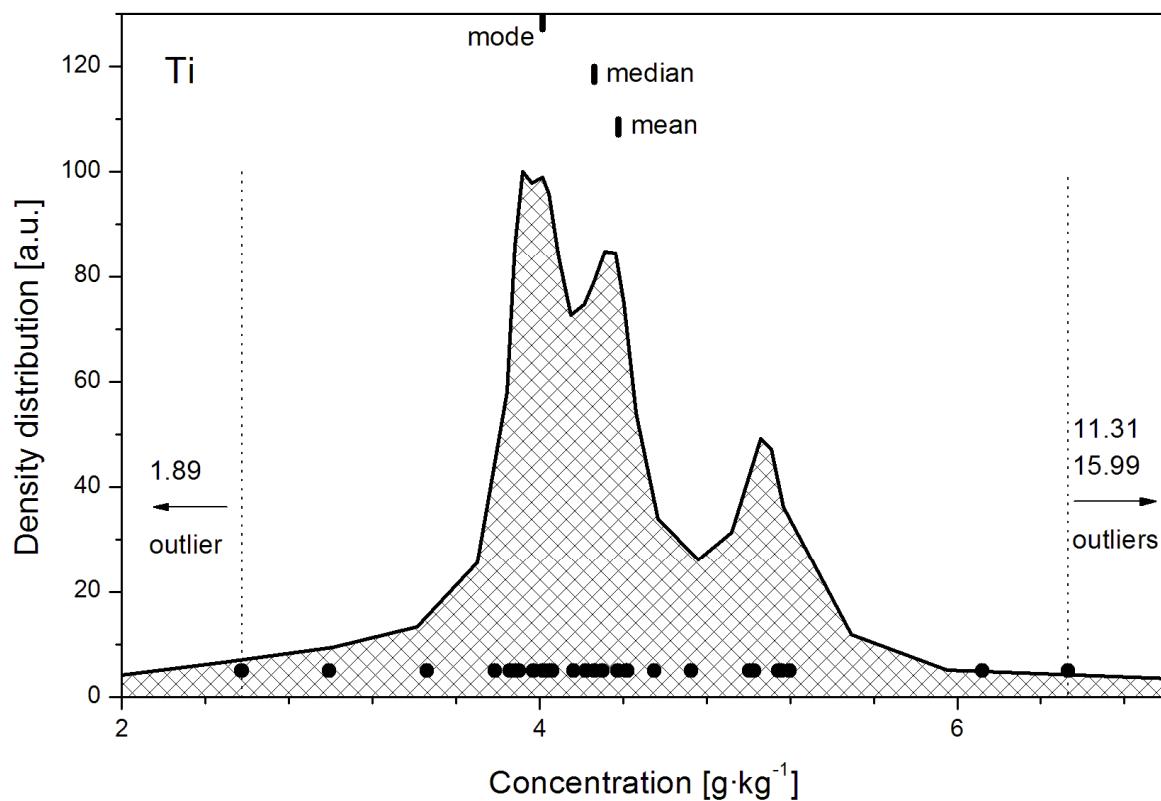


FIG. 29. The density distribution function for the analyte Ti.

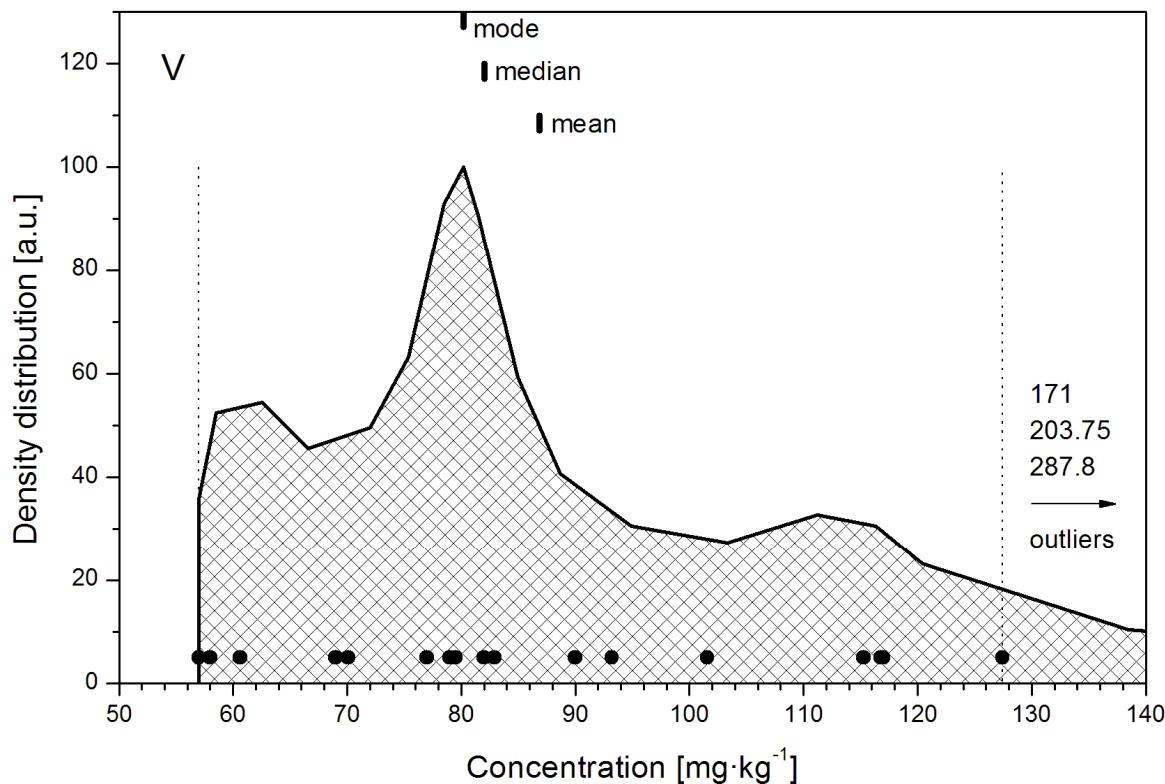


FIG. 30. The density distribution function for the analyte V.

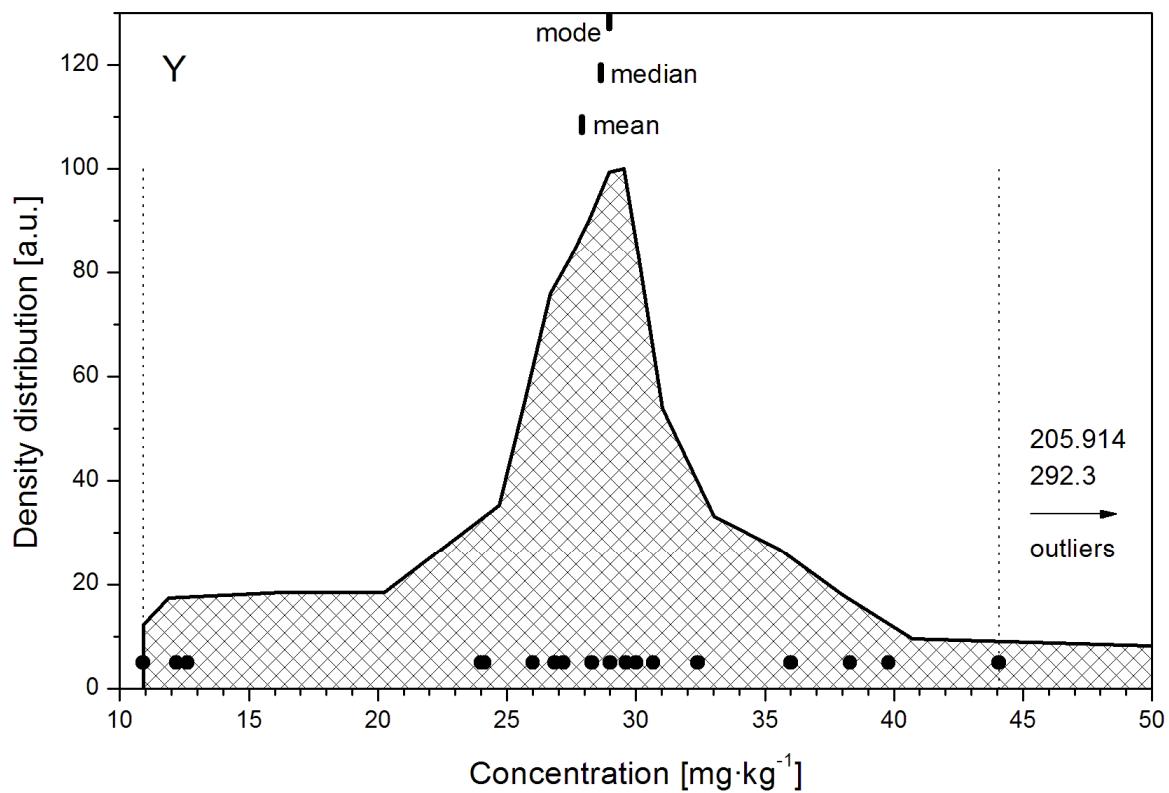


FIG. 31. The density distribution function for the analyte Y.

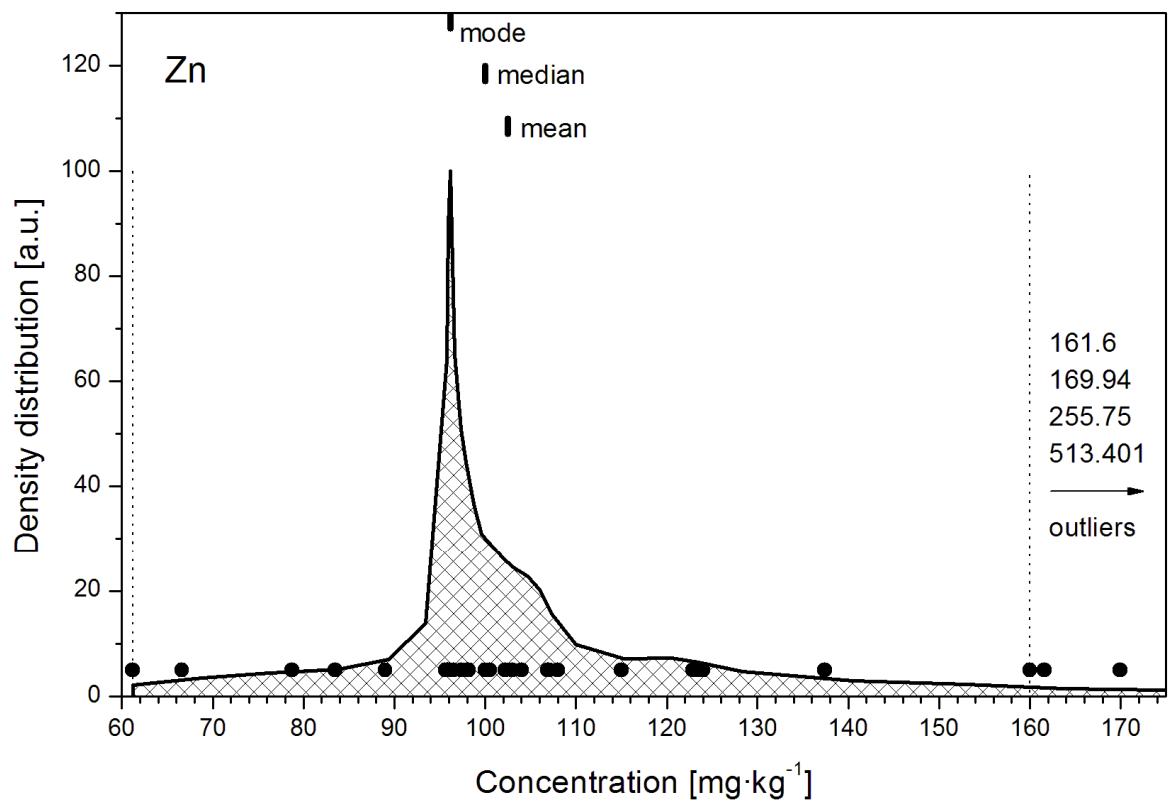


FIG. 32. The density distribution function for the analyte Zn.

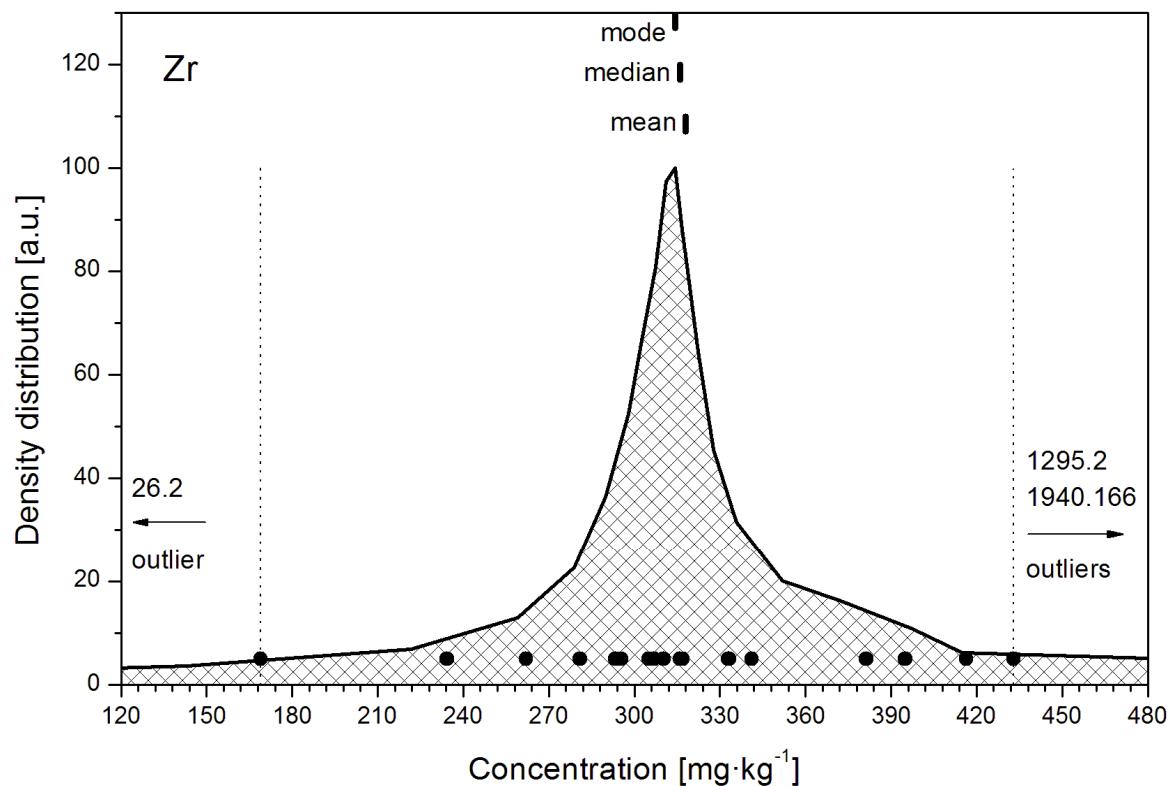


FIG. 33. The density distribution function for the analyte Zr.

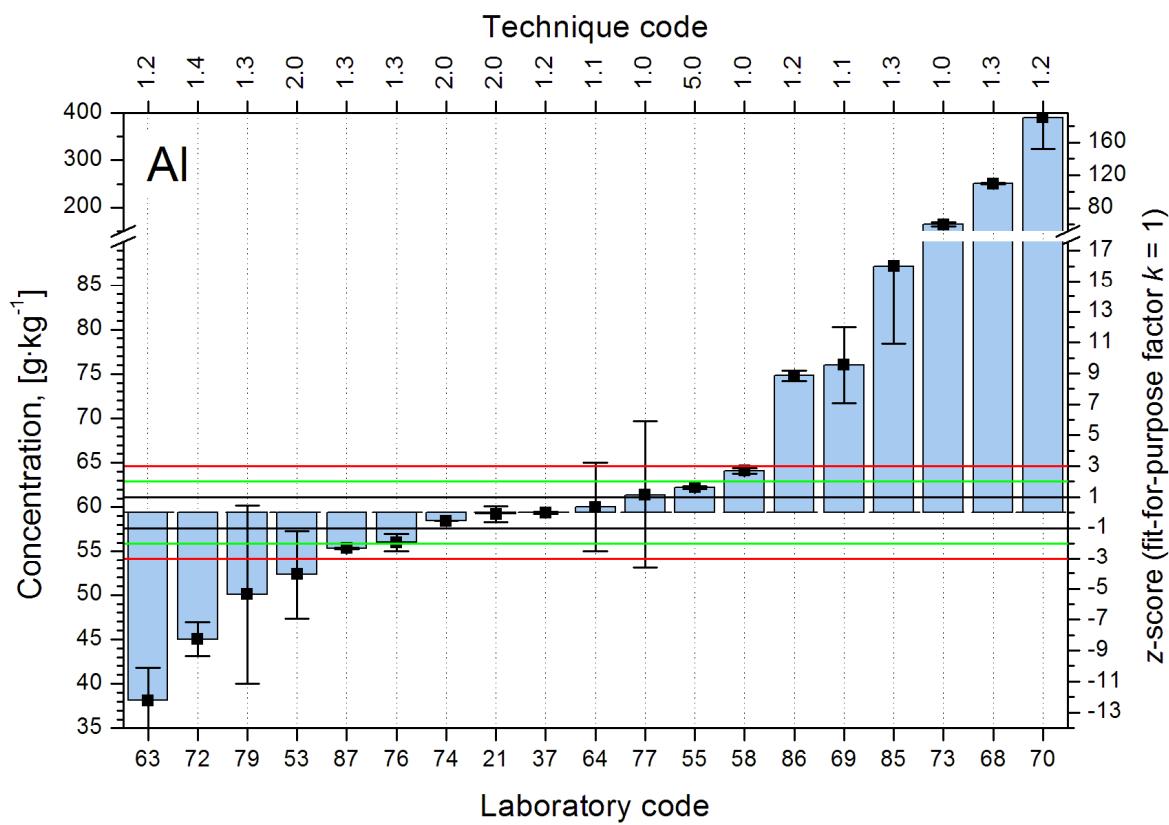


FIG. 34. Distributions of  $z$ -scores for analyte Al.

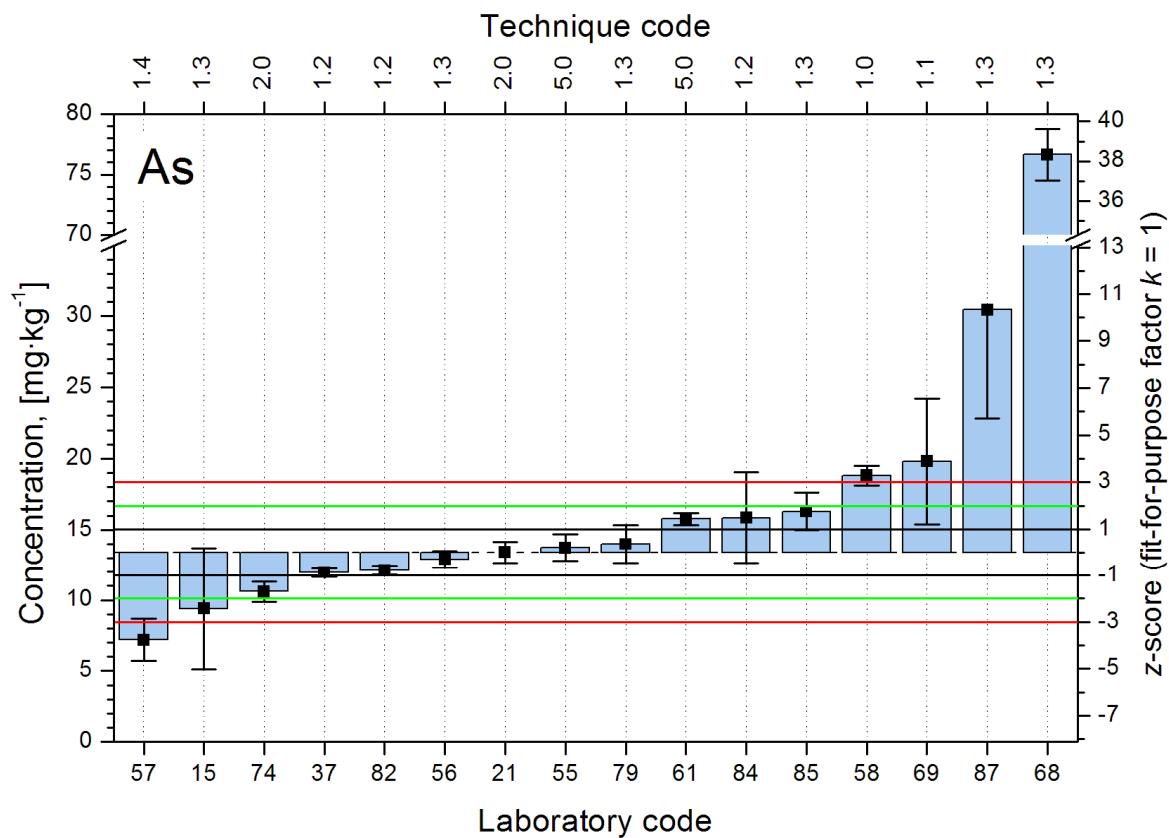


FIG. 35. Distributions of  $z$ -scores for analyte As.

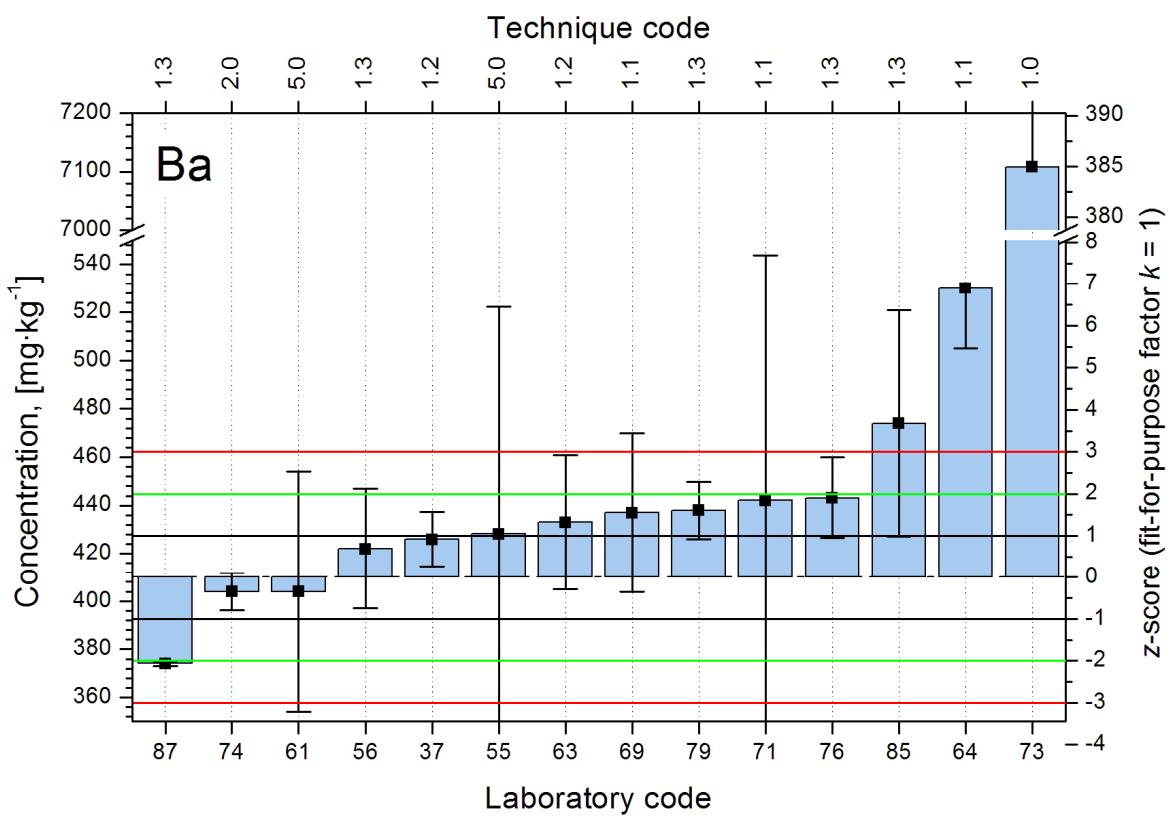


FIG. 36. Distributions of  $z$ -scores for analyte Ba.

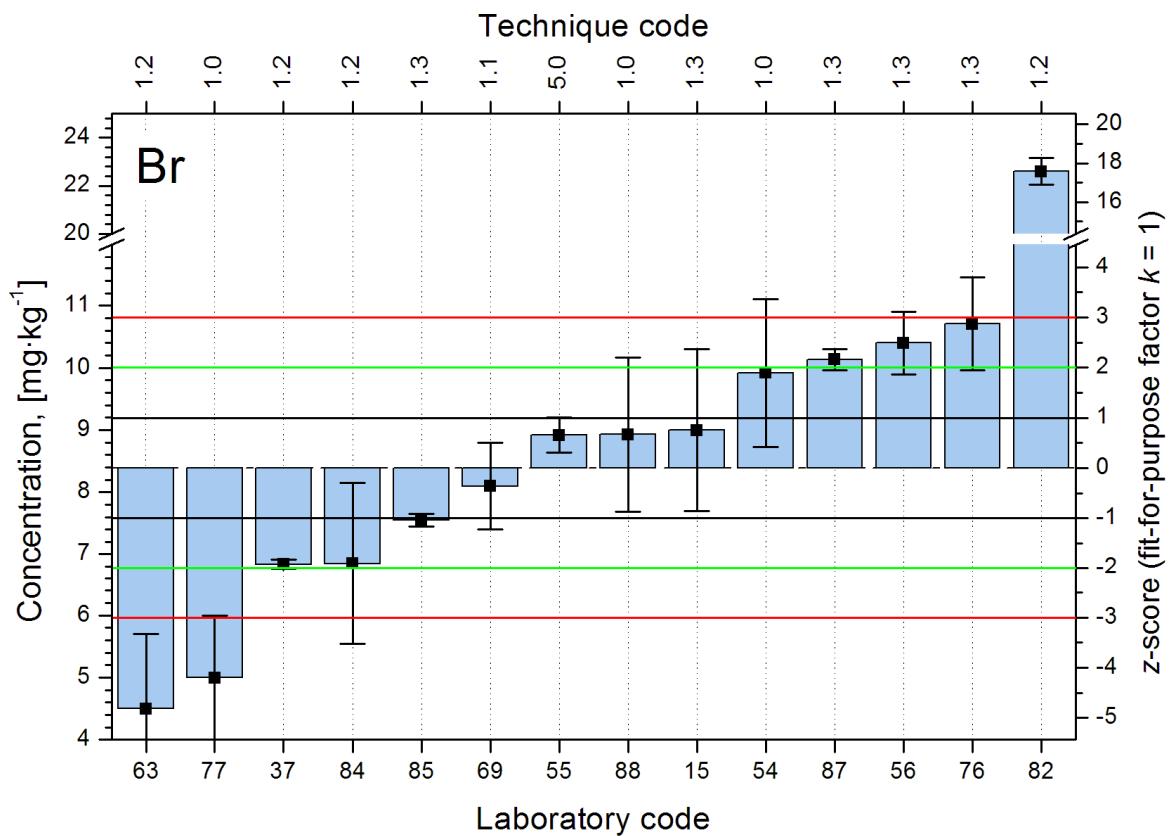


FIG. 37. Distributions of  $z$ -scores for analyte Br.

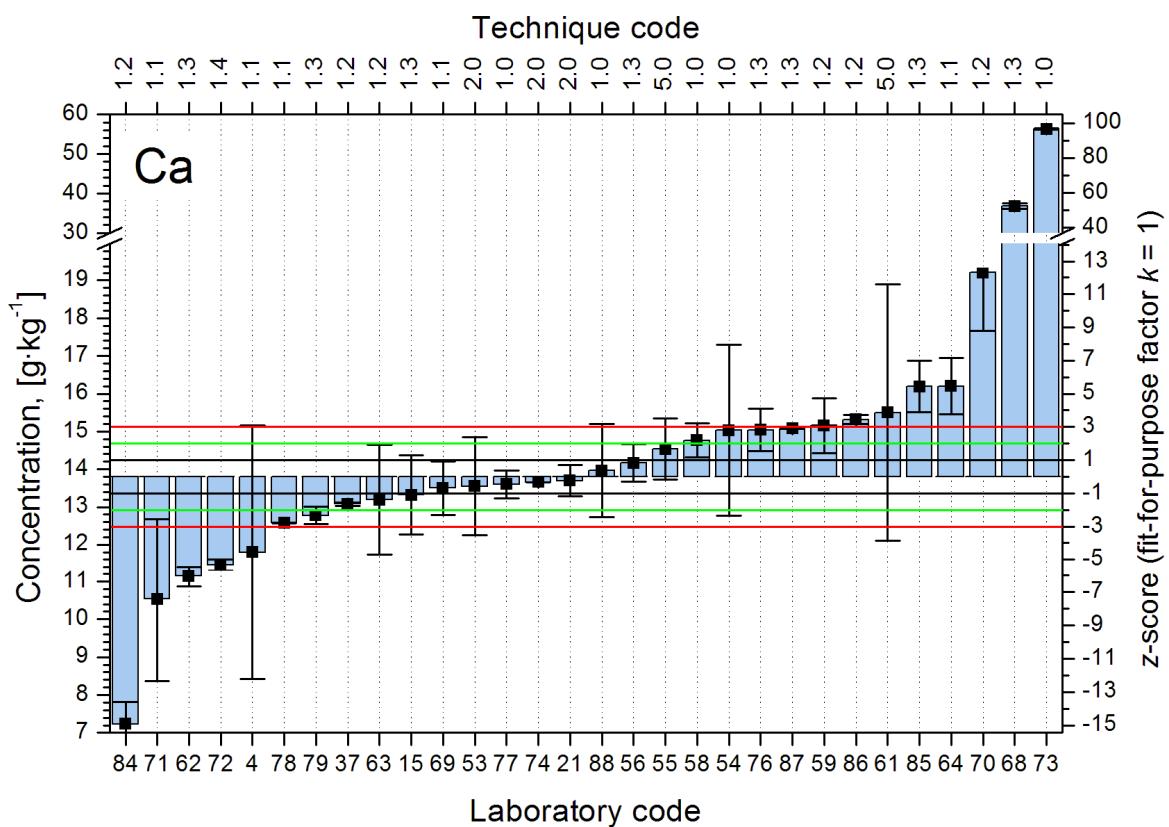


FIG. 38. Distributions of z-scores for analyte Ca.

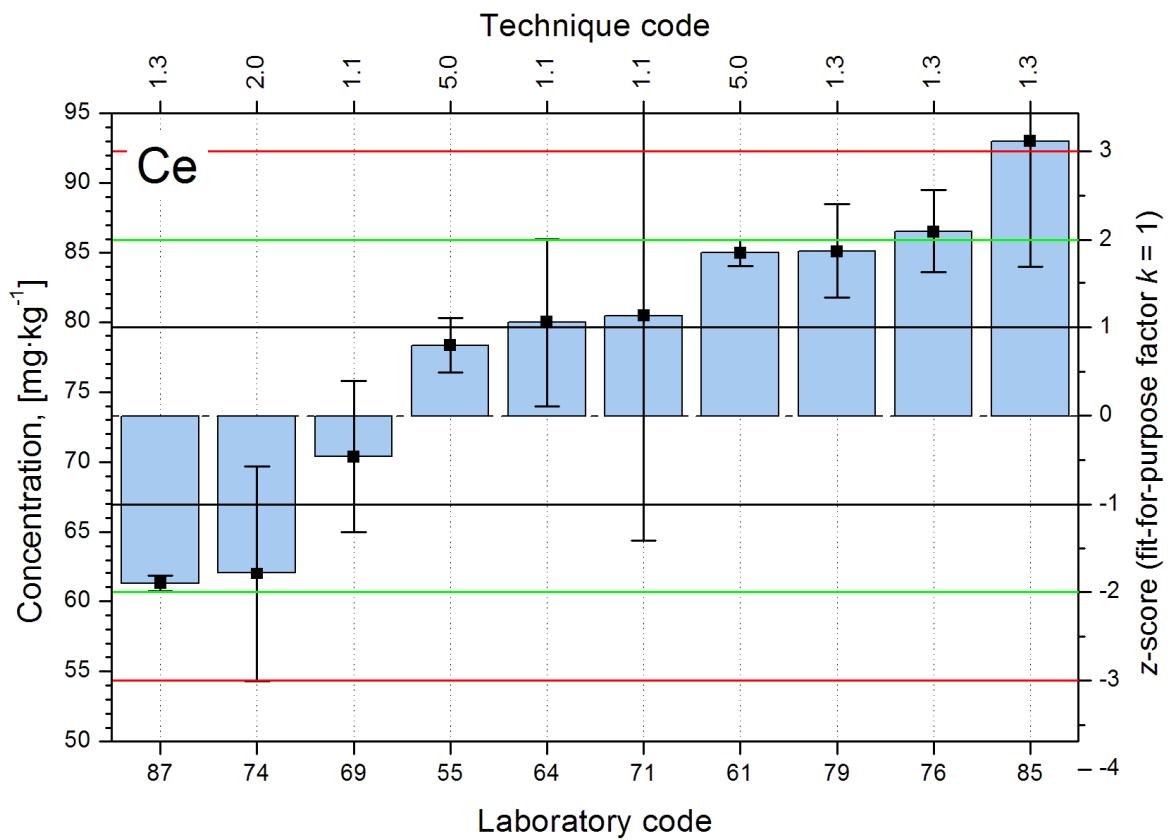


FIG. 39. Distributions of z-scores for analyte Ce.

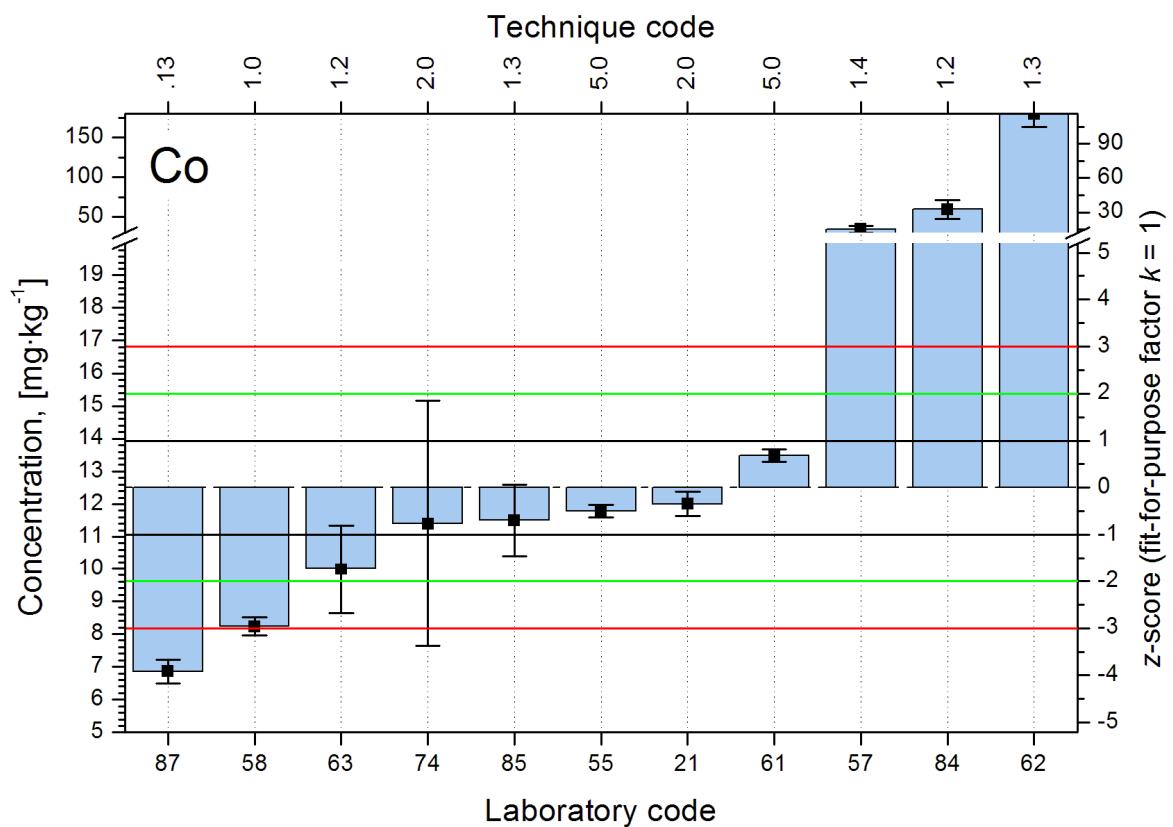


FIG. 40. Distributions of *z*-scores for analyte Co.

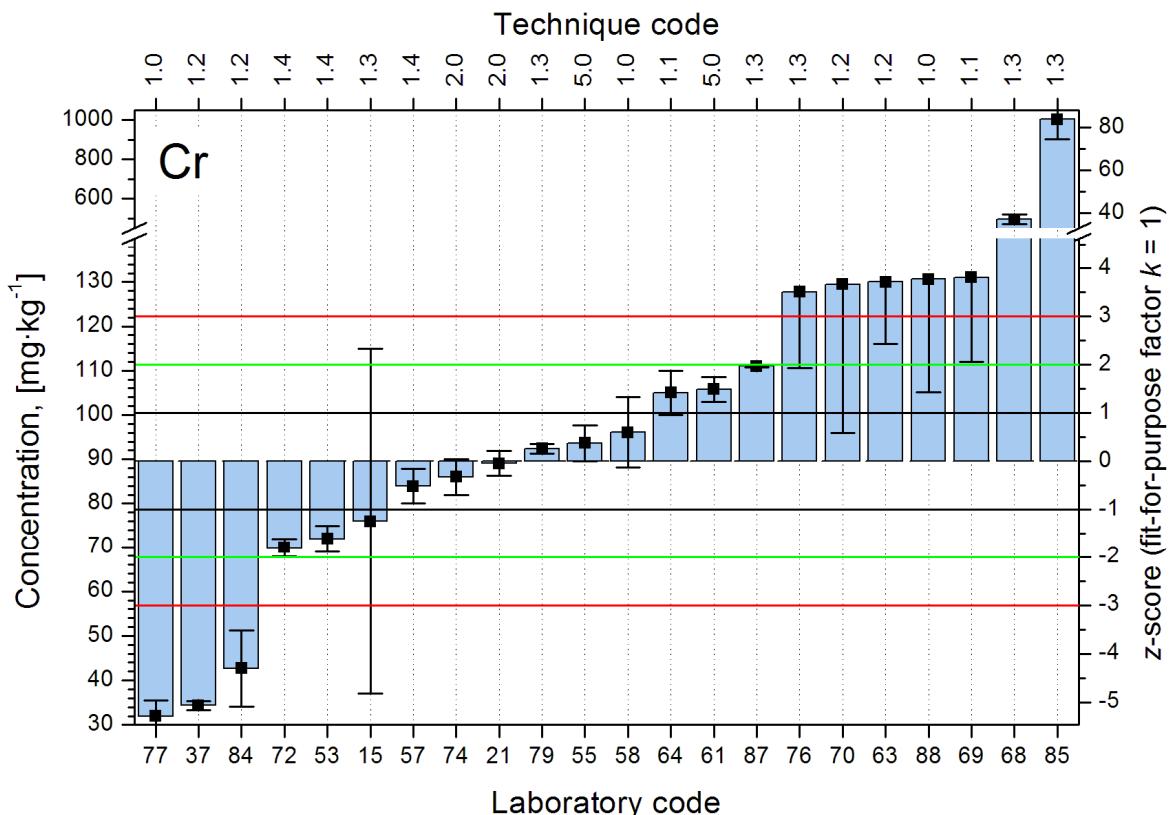


FIG. 41. Distributions of *z*-scores for analyte Cr.

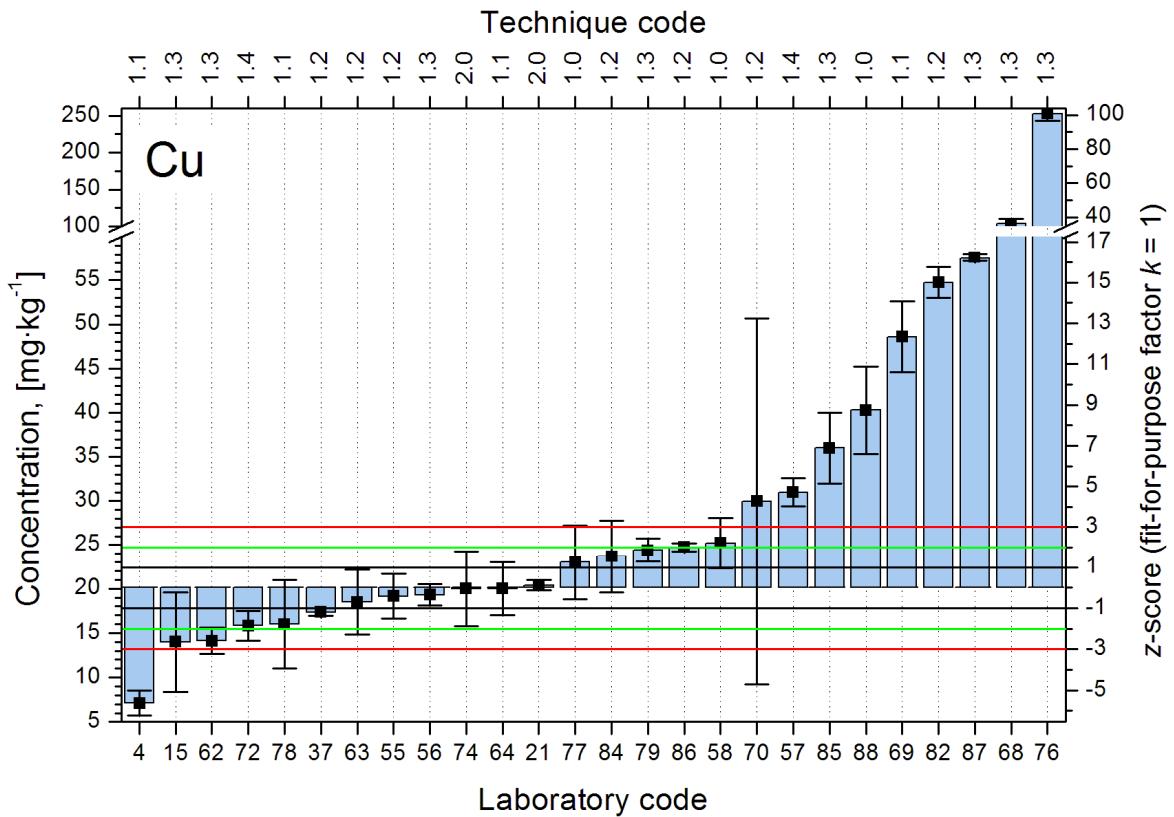


FIG. 42. Distributions of  $z$ -scores for analyte Cu.

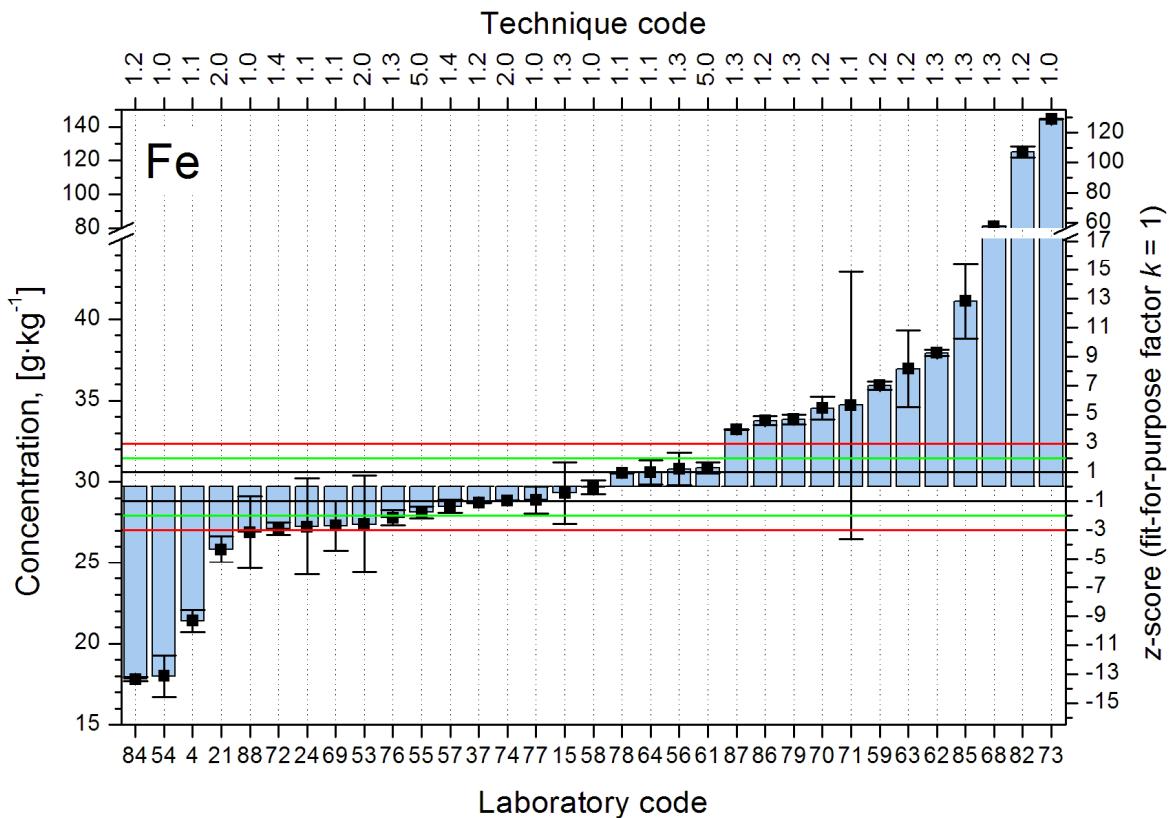


FIG. 43. Distributions of  $z$ -scores for analyte Fe.

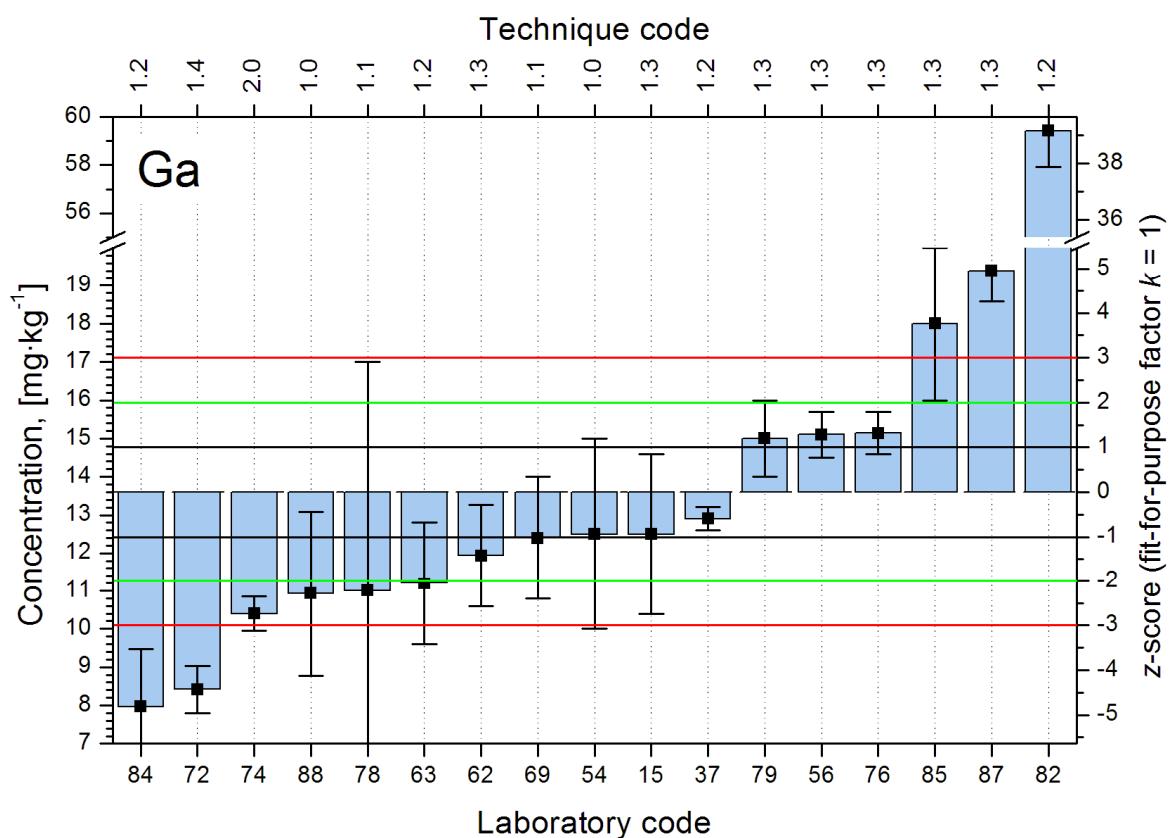


FIG. 44. Distributions of  $z$ -scores for analyte Ga.

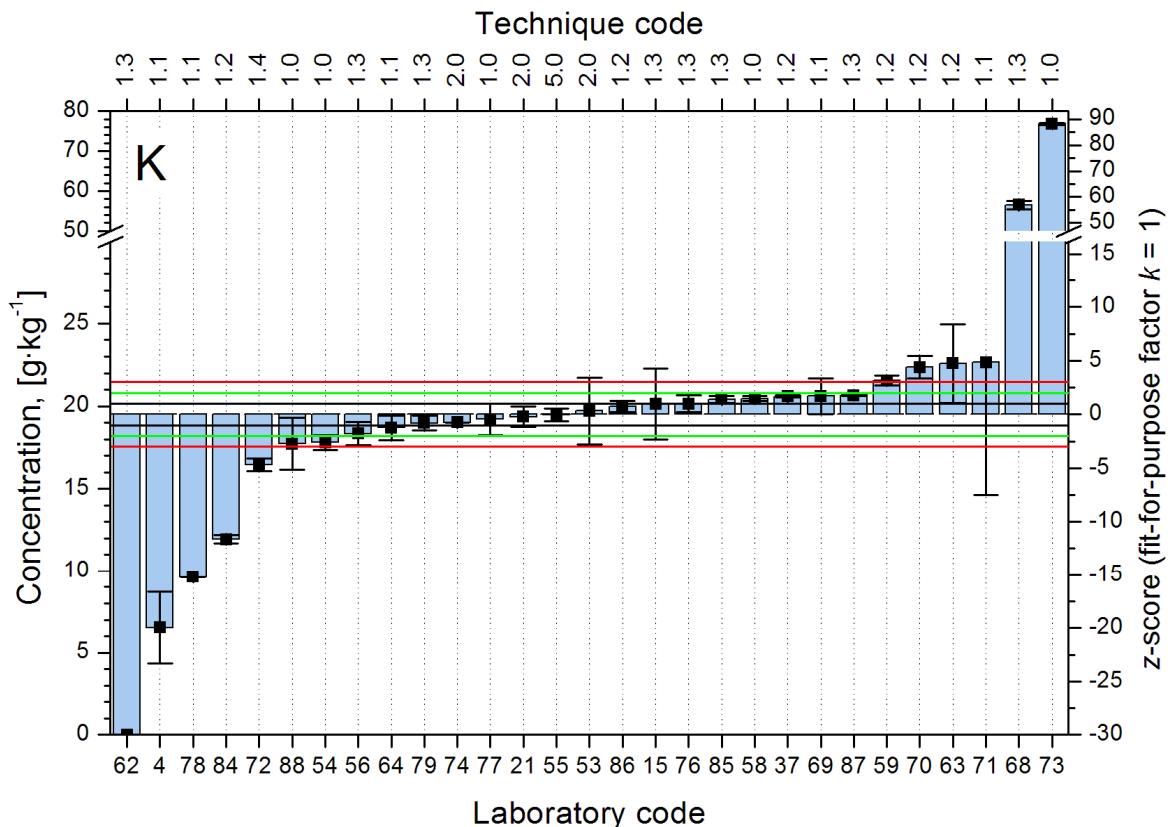


FIG. 45. Distributions of  $z$ -scores for analyte K.

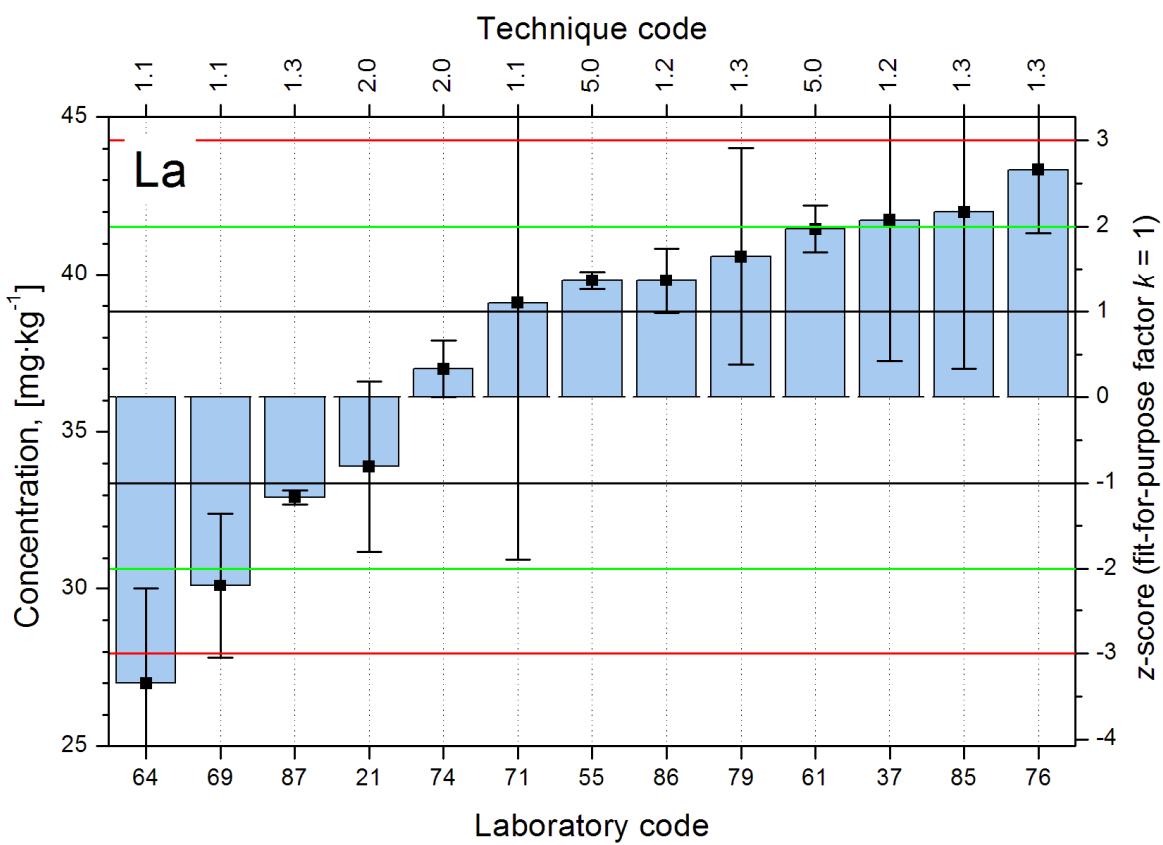


FIG. 46. Distributions of  $z$ -scores for analyte La.

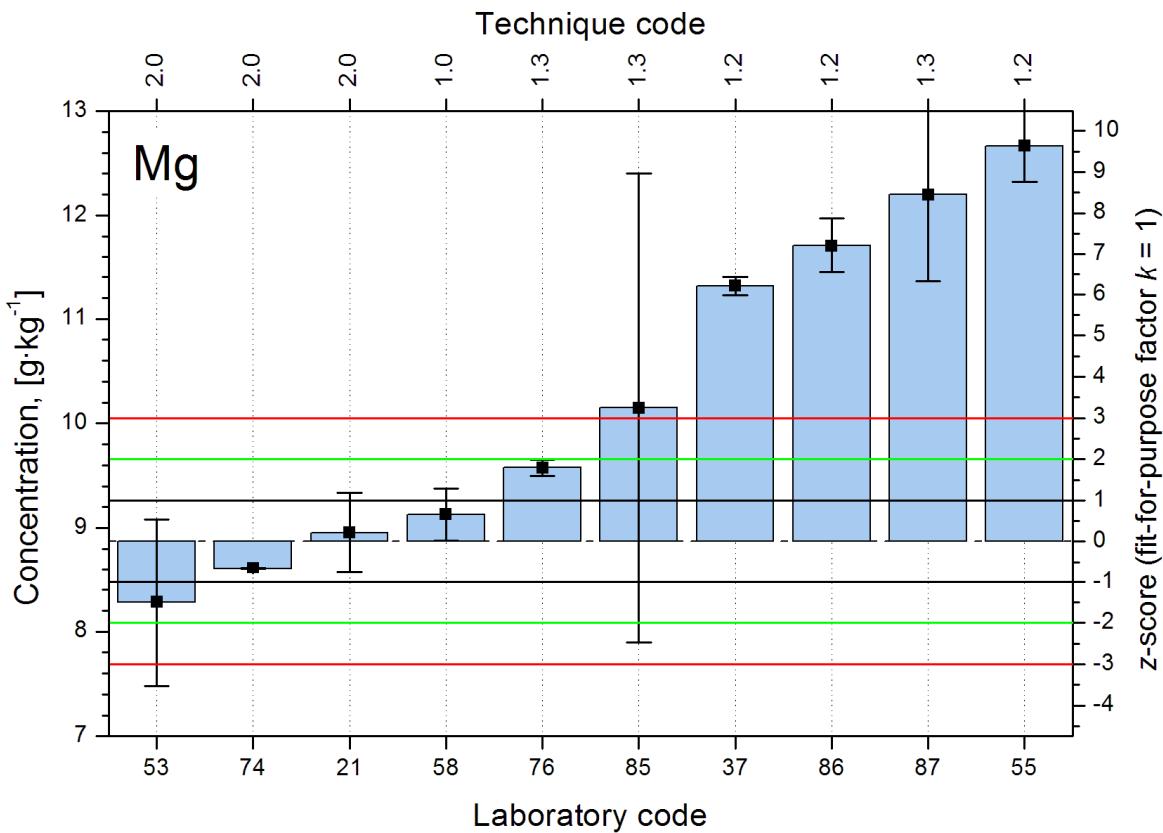


FIG. 47. Distributions of  $z$ -scores for analyte Mg.

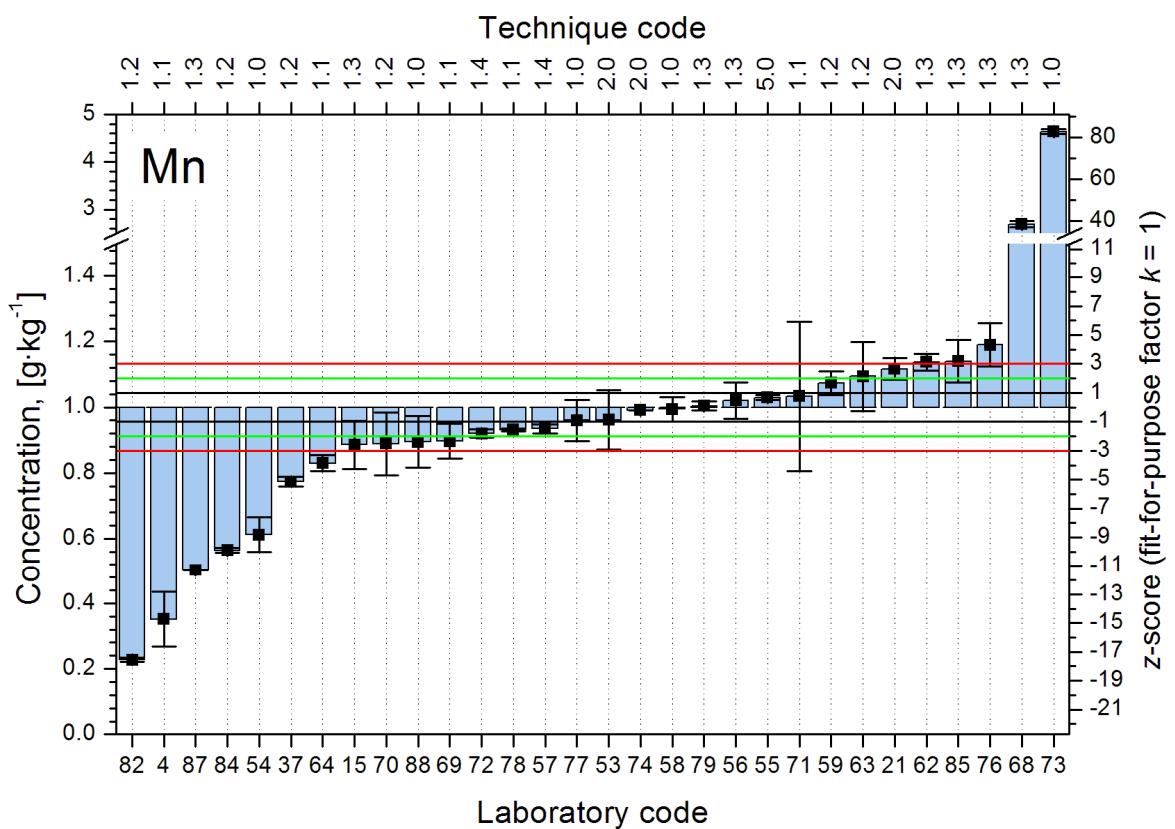


FIG. 48. Distributions of  $z$ -scores for analyte Mn.

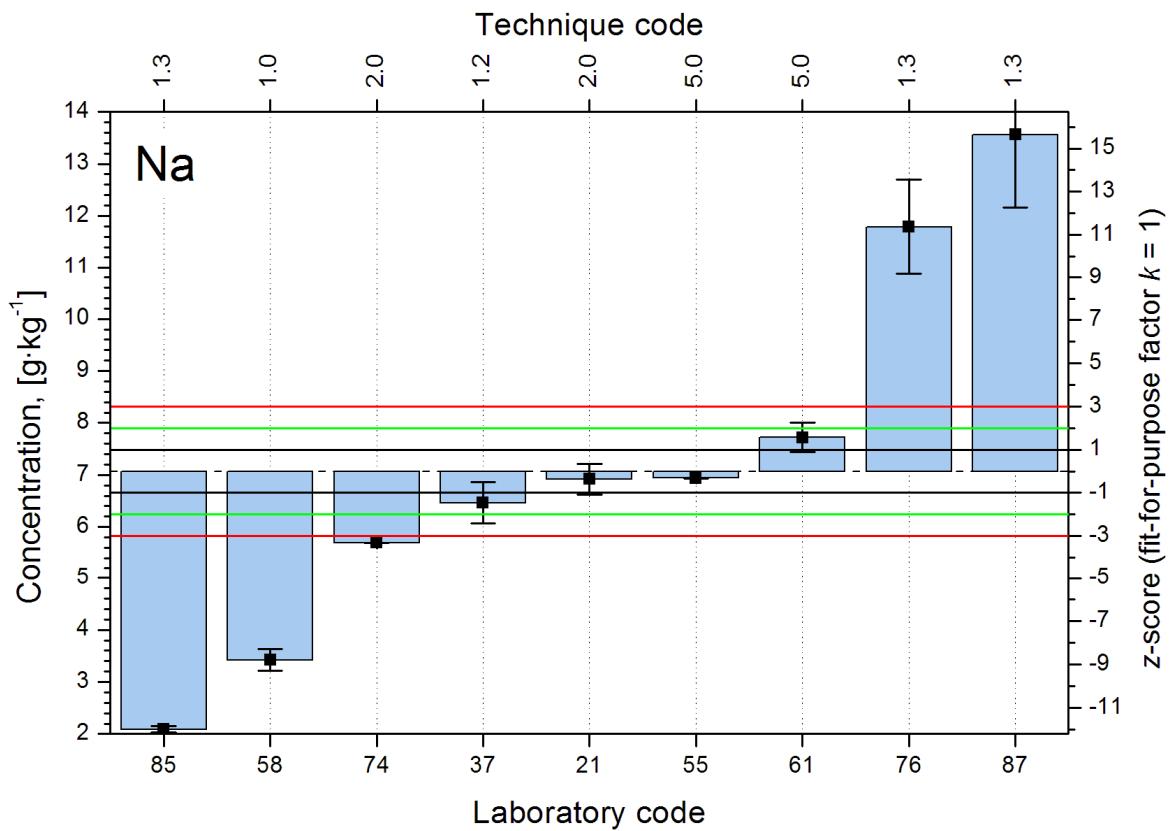


FIG. 49. Distributions of  $z$ -scores for analyte Na.

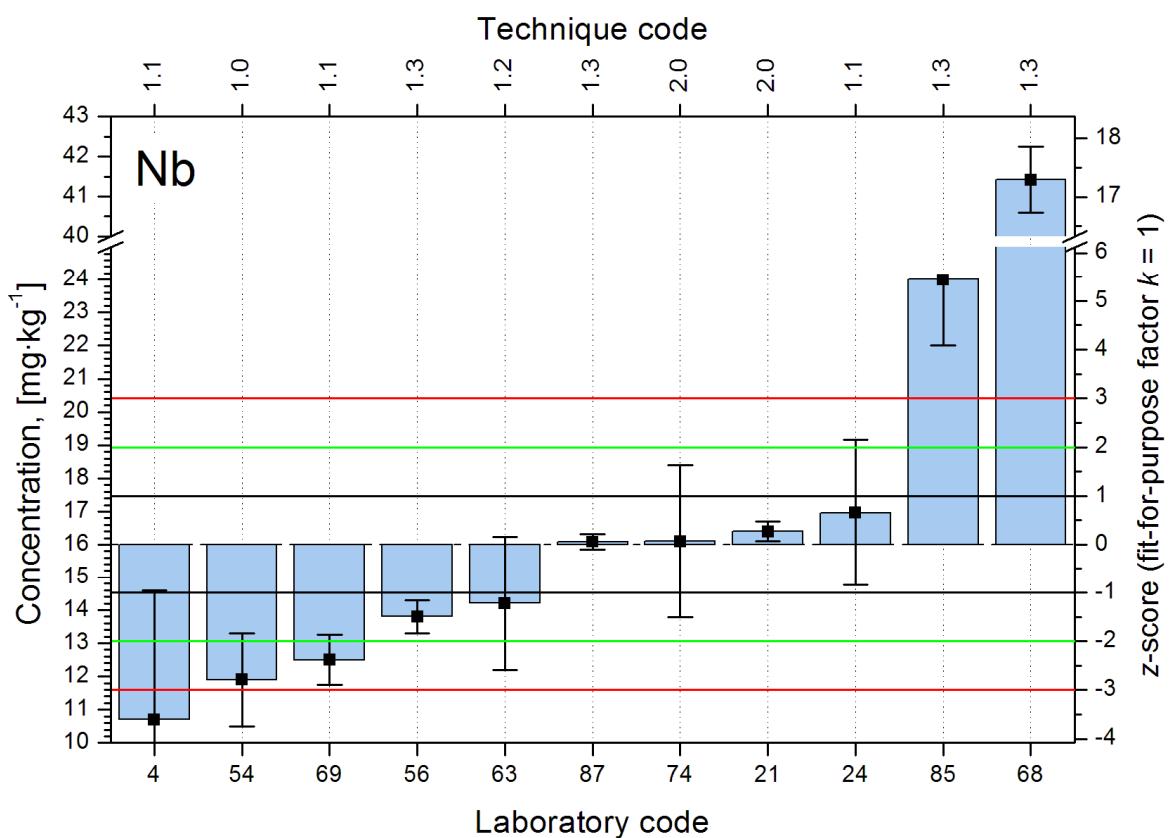


FIG. 50. Distributions of  $z$ -scores for analyte Nb.

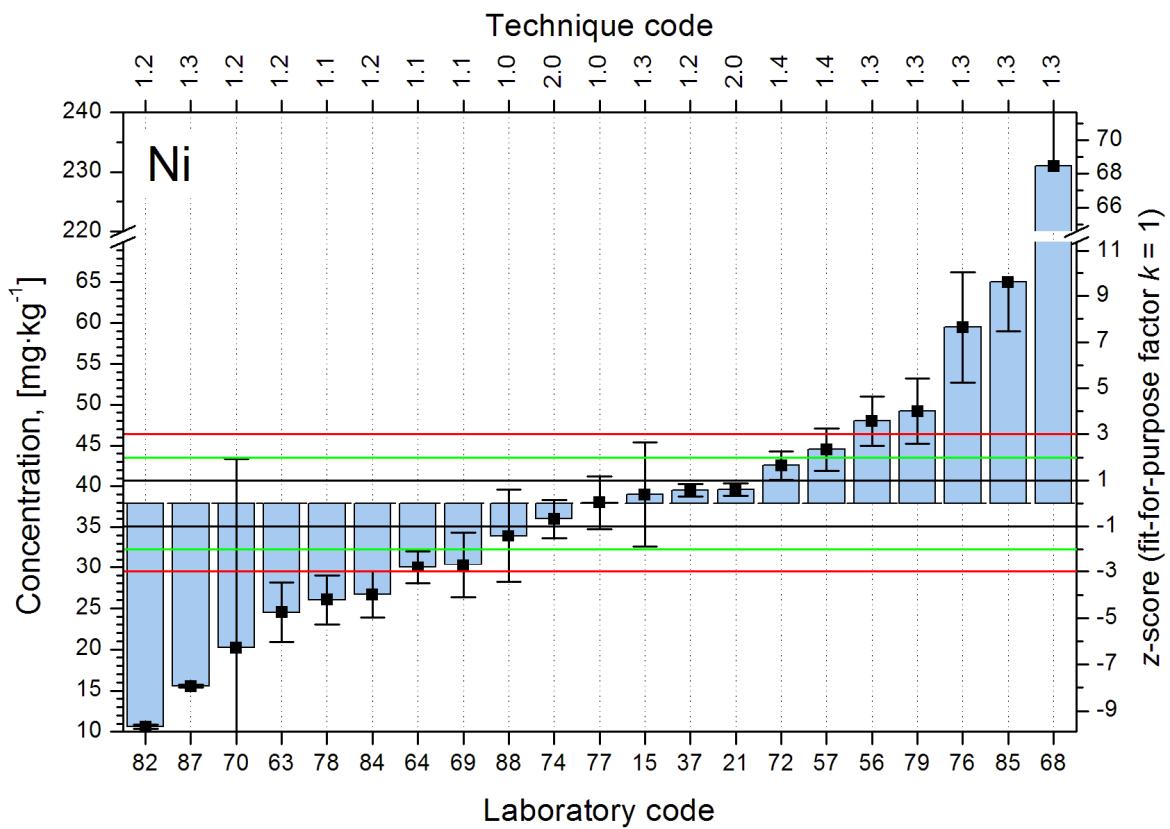


FIG. 51. Distributions of  $z$ -scores for analyte Ni.

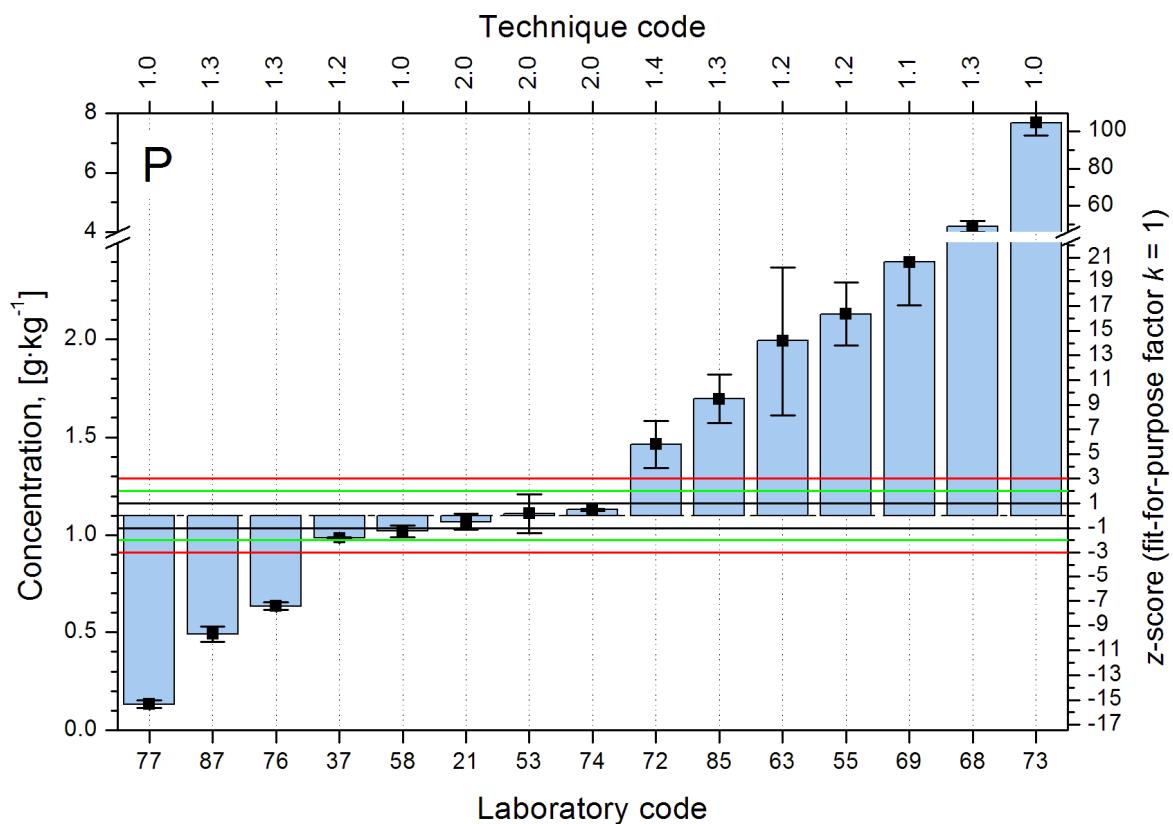


FIG. 52. Distributions of  $z$ -scores for analyte  $P$ .

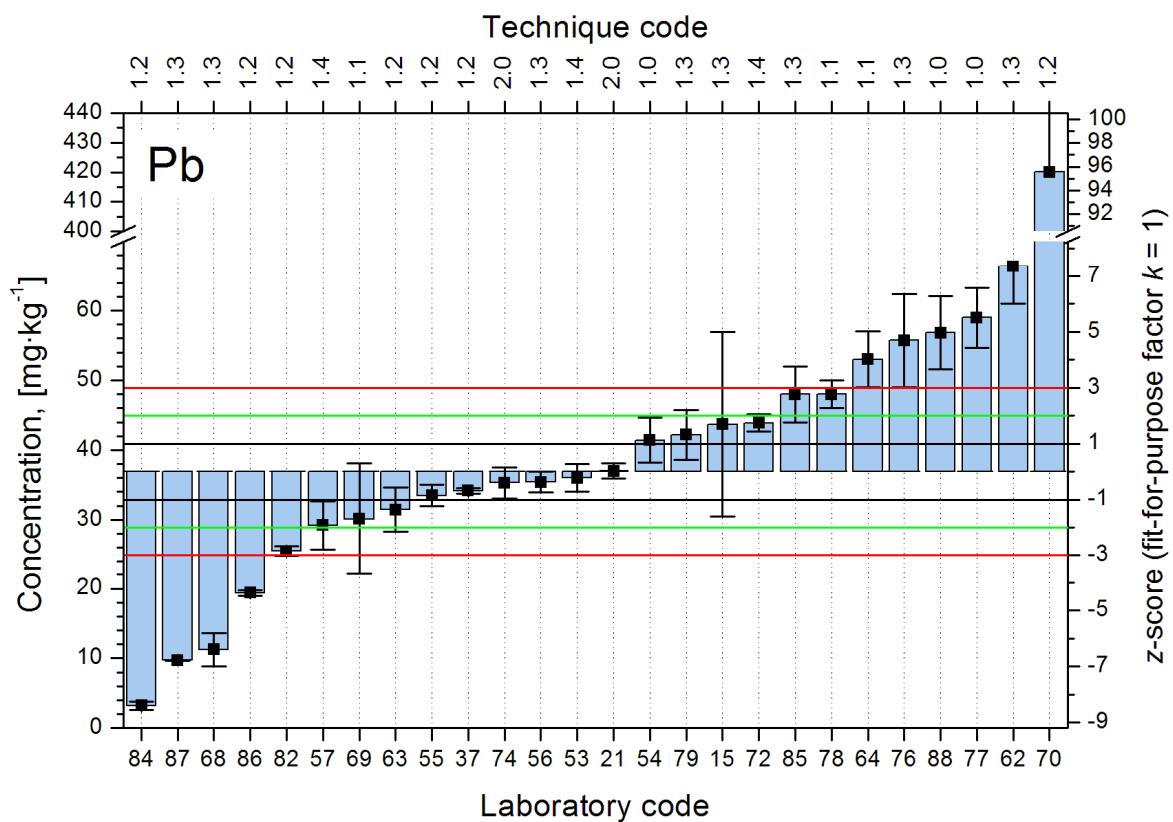


FIG. 53. Distributions of  $z$ -scores for analyte  $Pb$ .

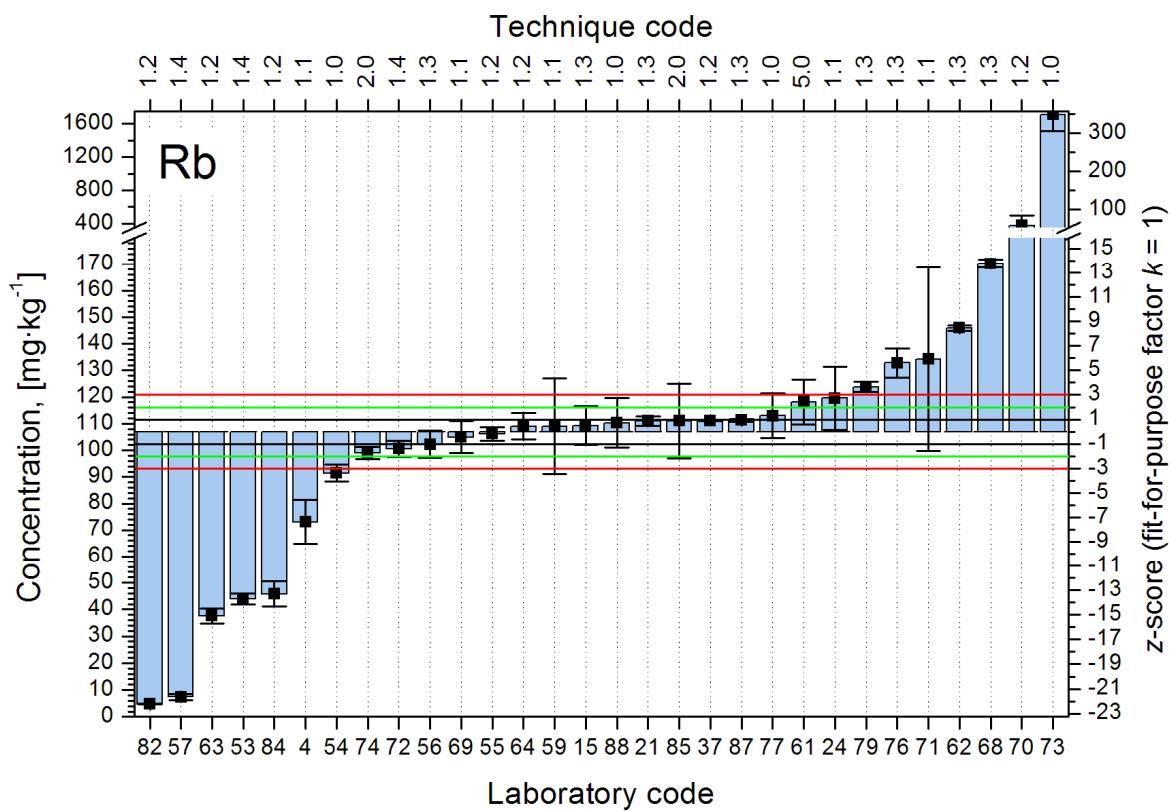


FIG. 54. Distributions of z-scores for analyte Rb.

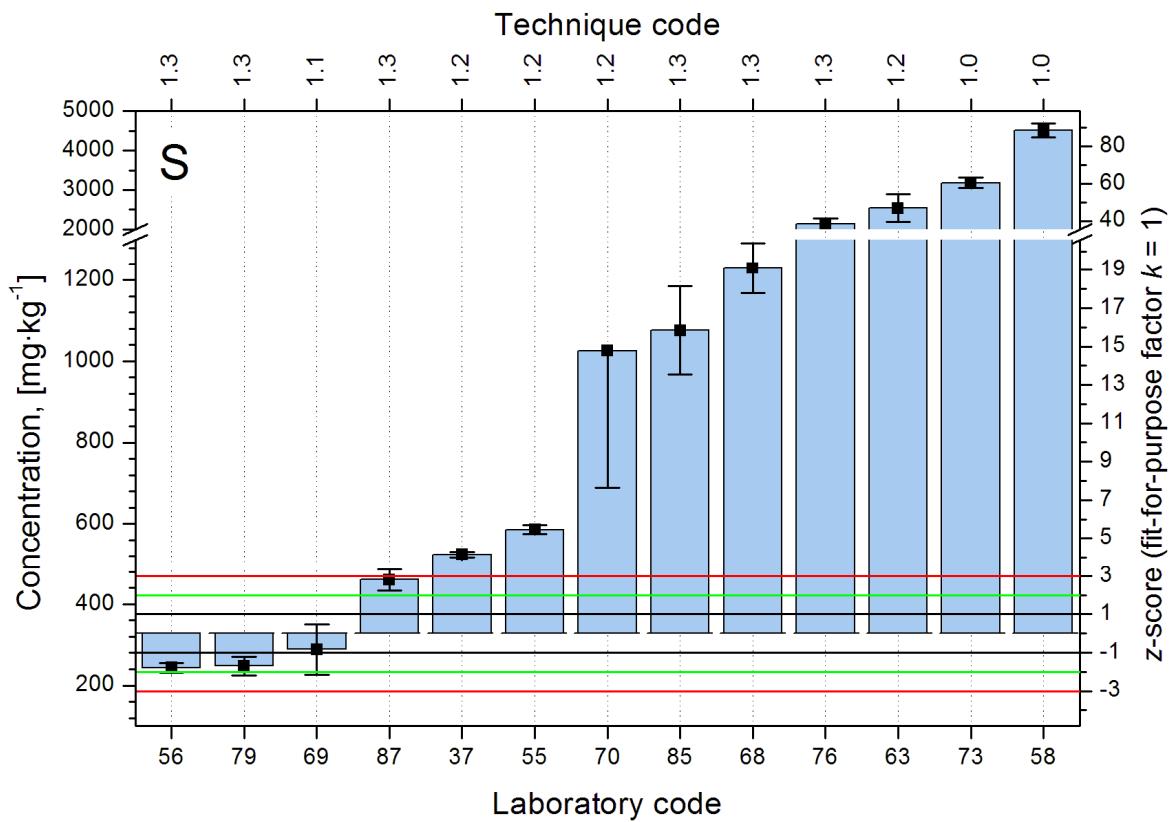


FIG. 55. Distributions of z-scores for analyte S.

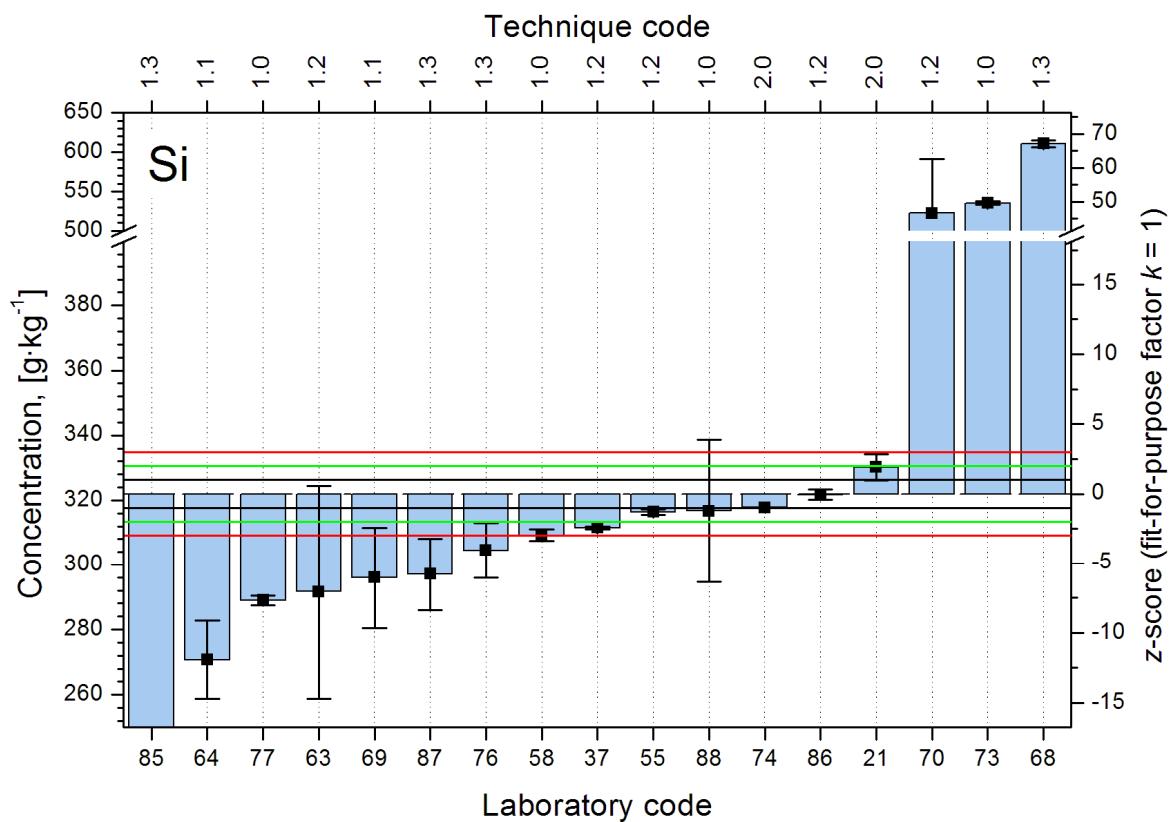


FIG. 56. Distributions of  $z$ -scores for analyte Si.

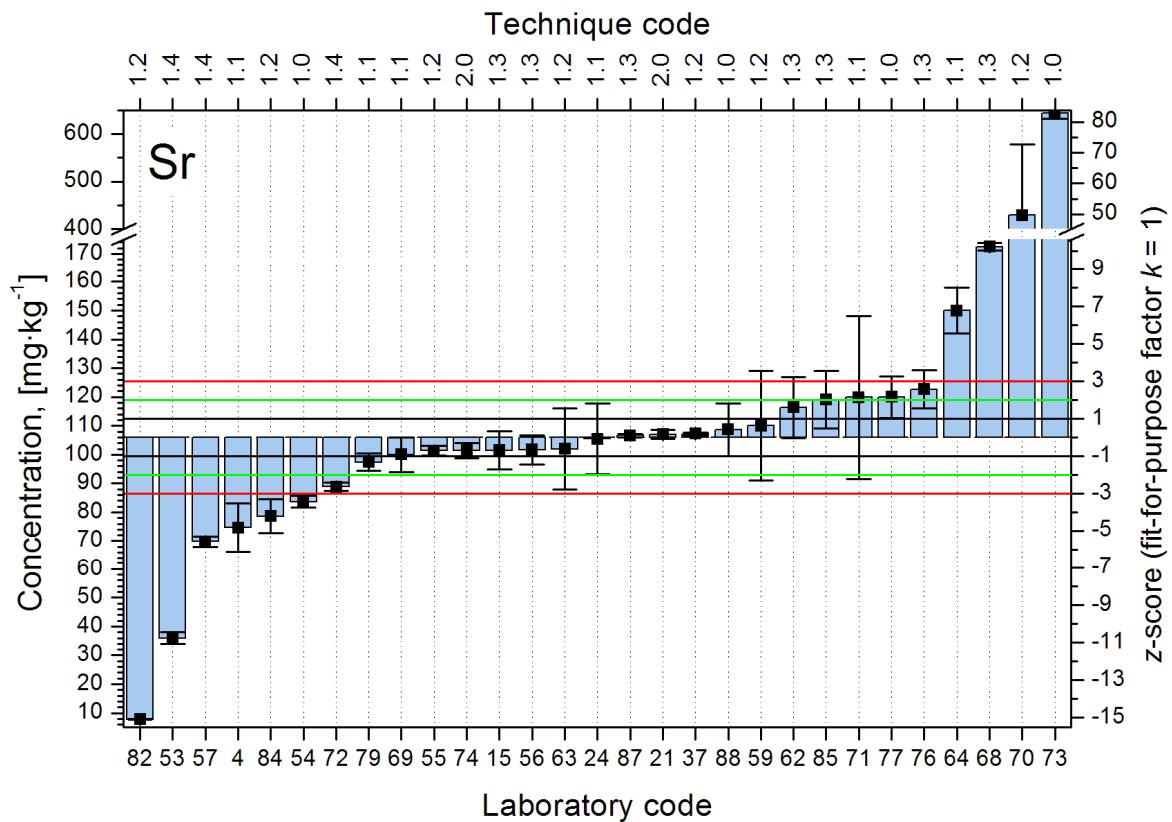


FIG. 57. Distributions of  $z$ -scores for analyte Sr.

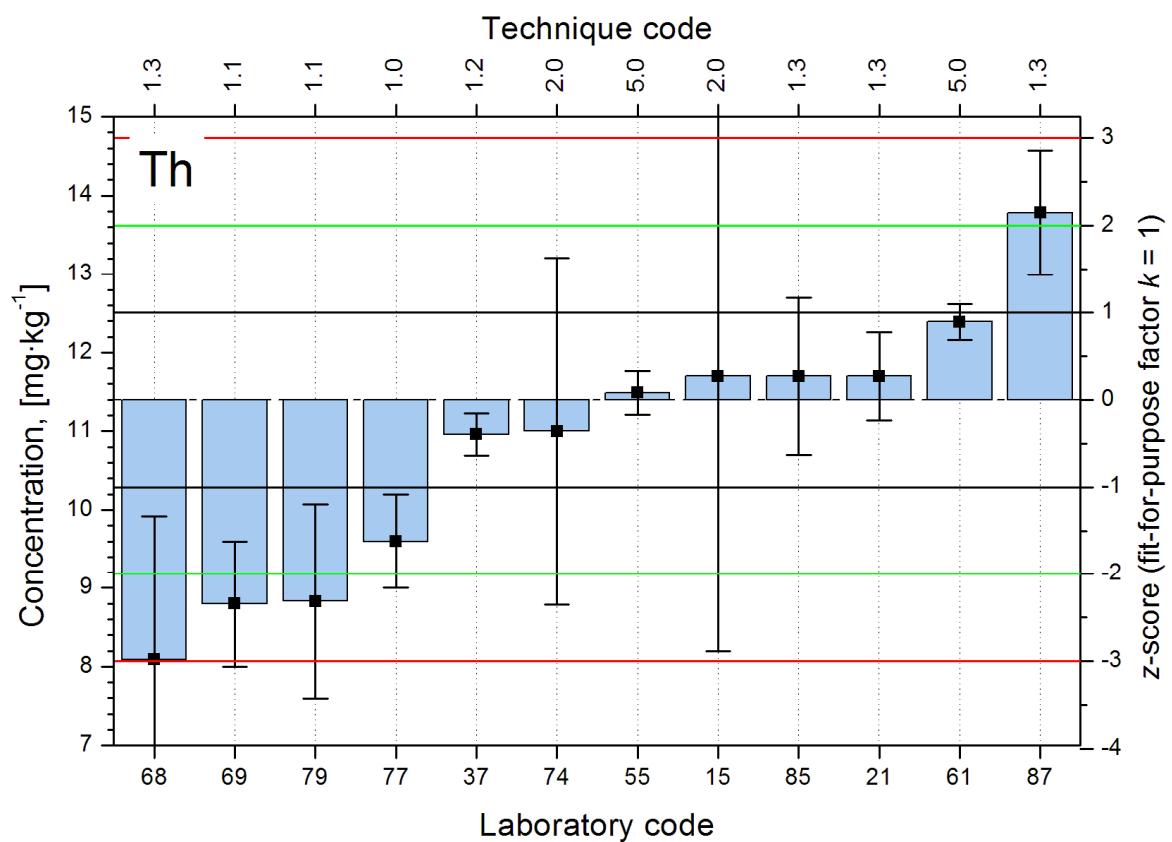


FIG. 58. Distributions of  $z$ -scores for analyte Th.

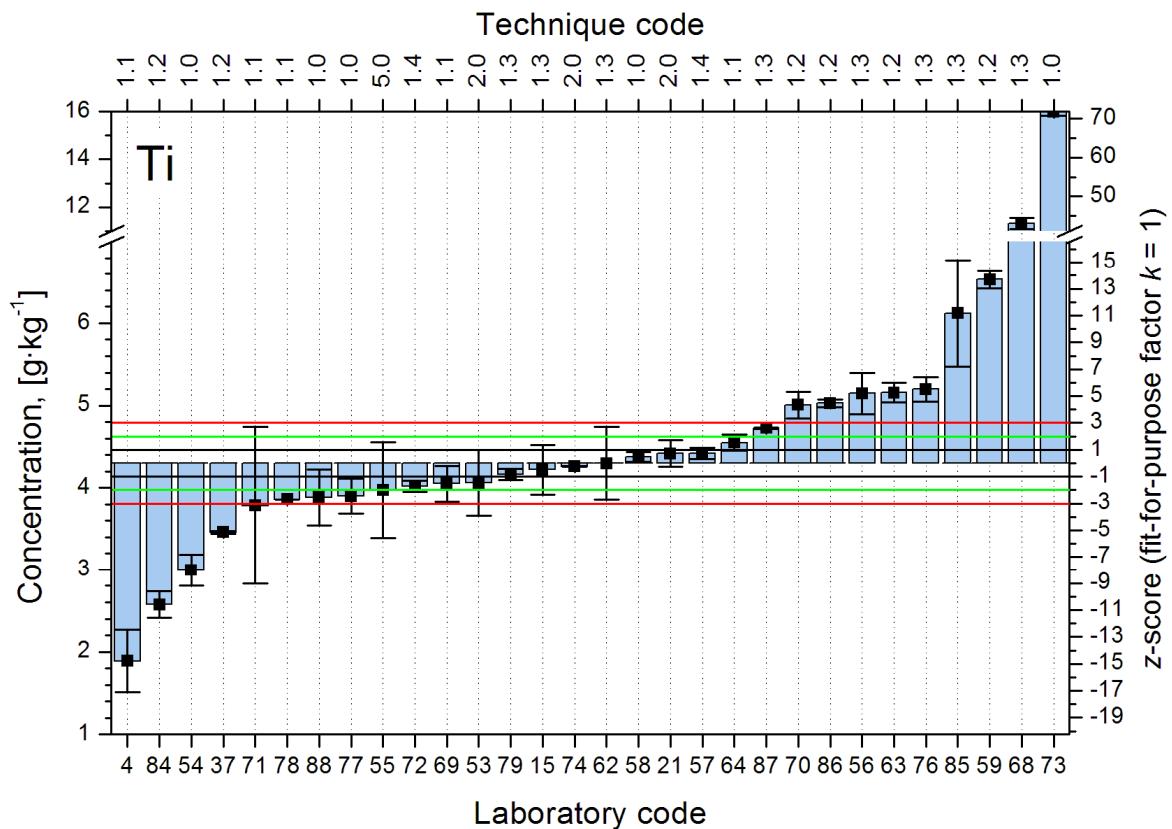


FIG. 59. Distributions of  $z$ -scores for analyte Ti.

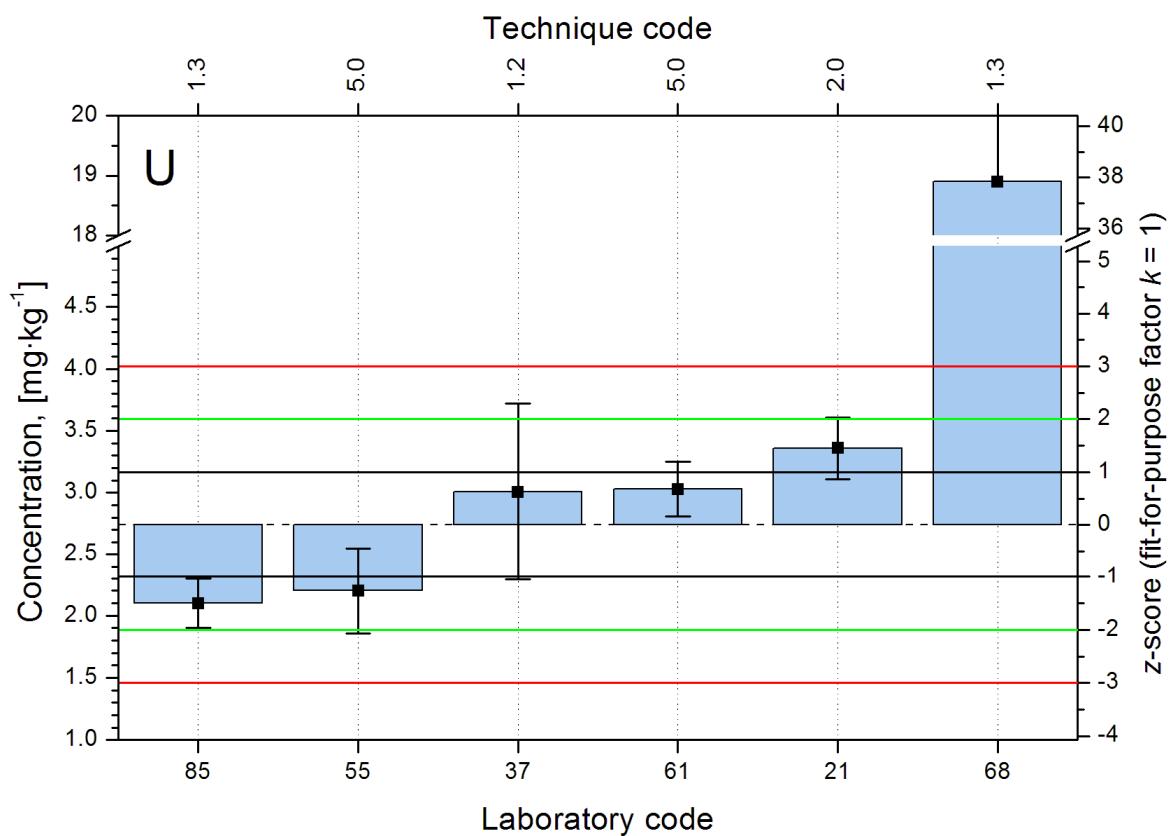


FIG. 60. Distributions of *z*-scores for analyte *U*.

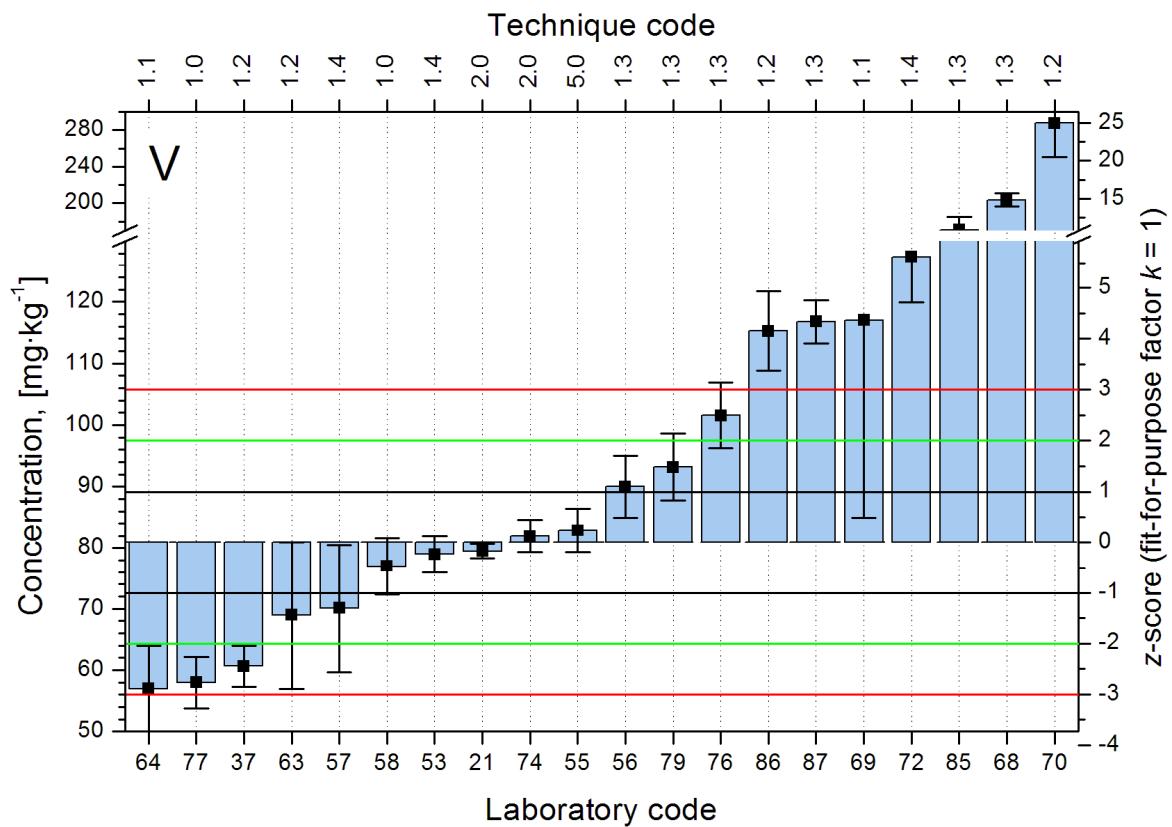


FIG. 61. Distributions of *z*-scores for analyte *V*.

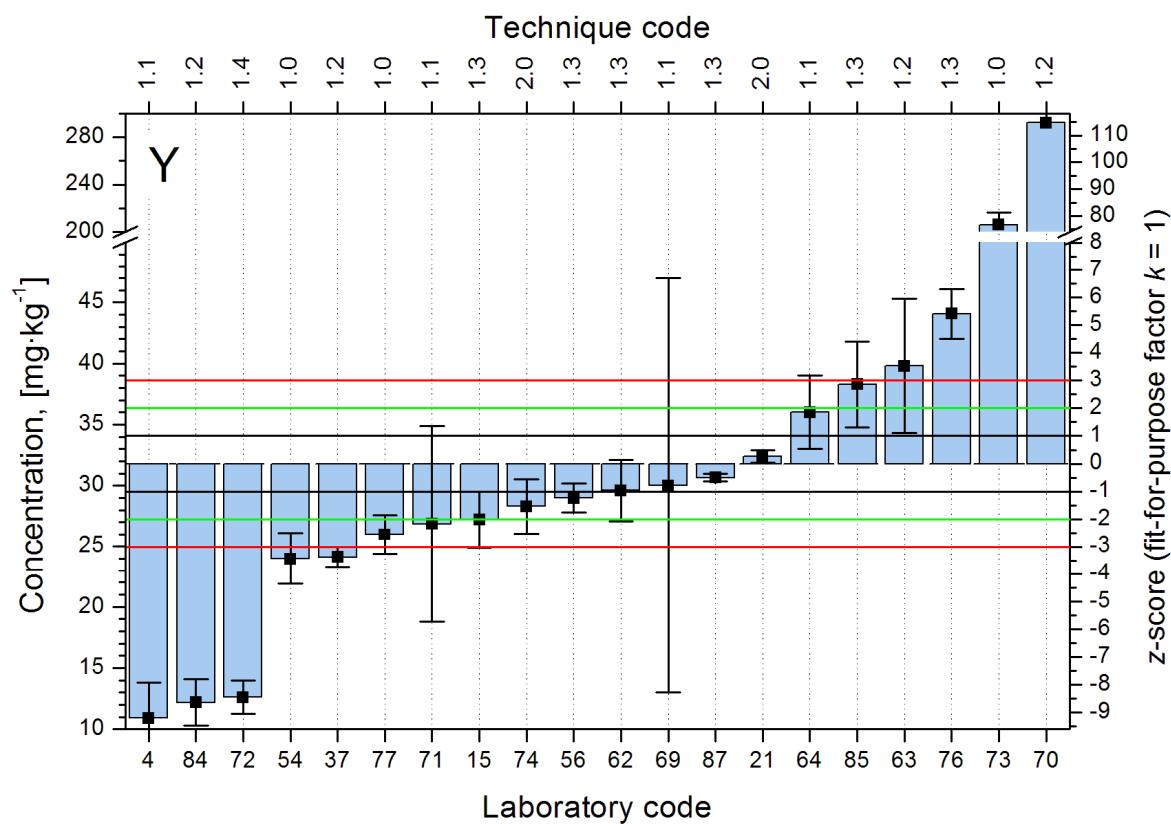


FIG. 62. Distributions of *z*-scores for analyte *Y*.

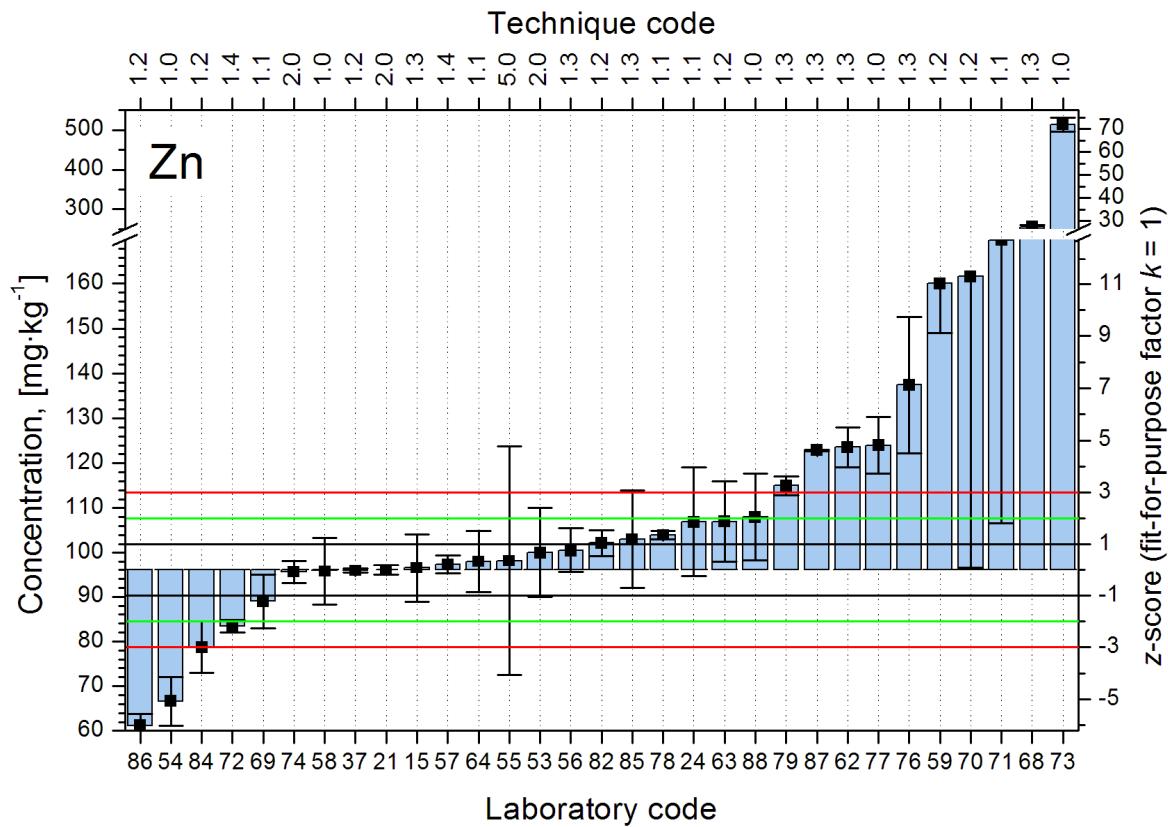


FIG. 63. Distributions of *z*-scores for analyte Zn.

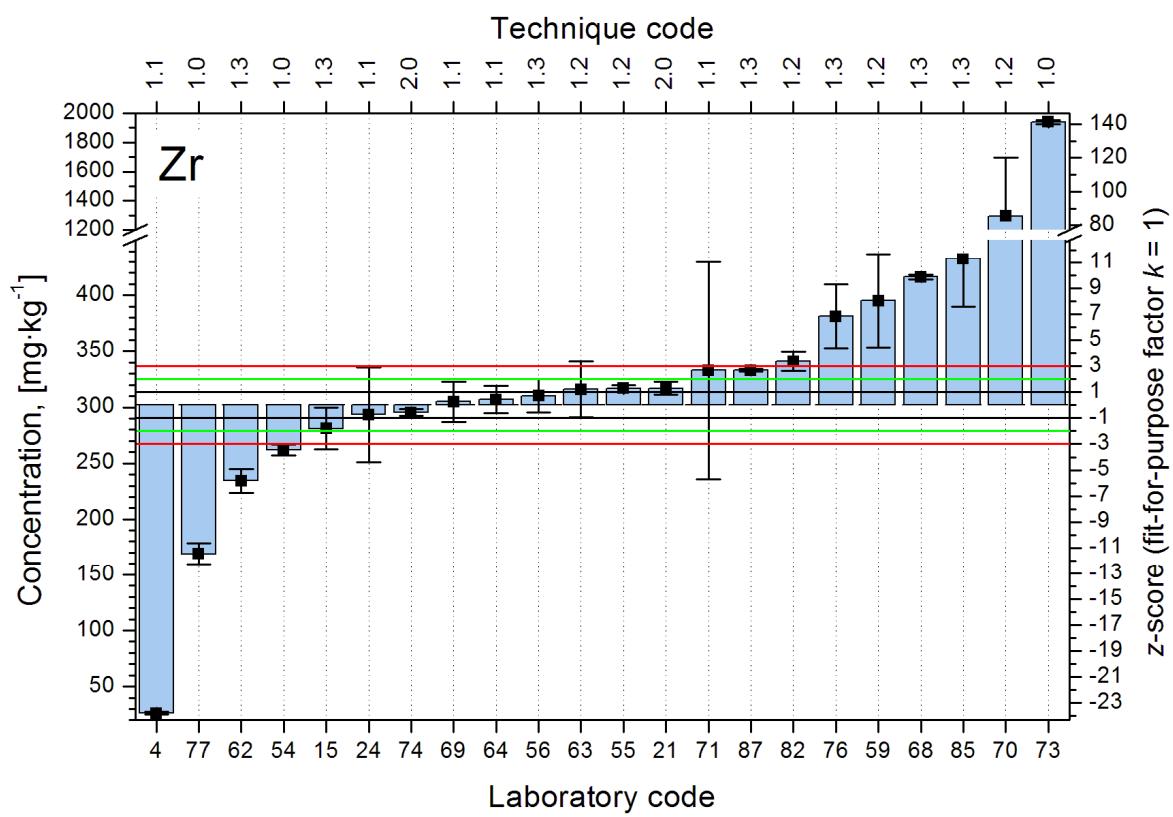


FIG. 64. Distributions of *z*-scores for analyte Zr.

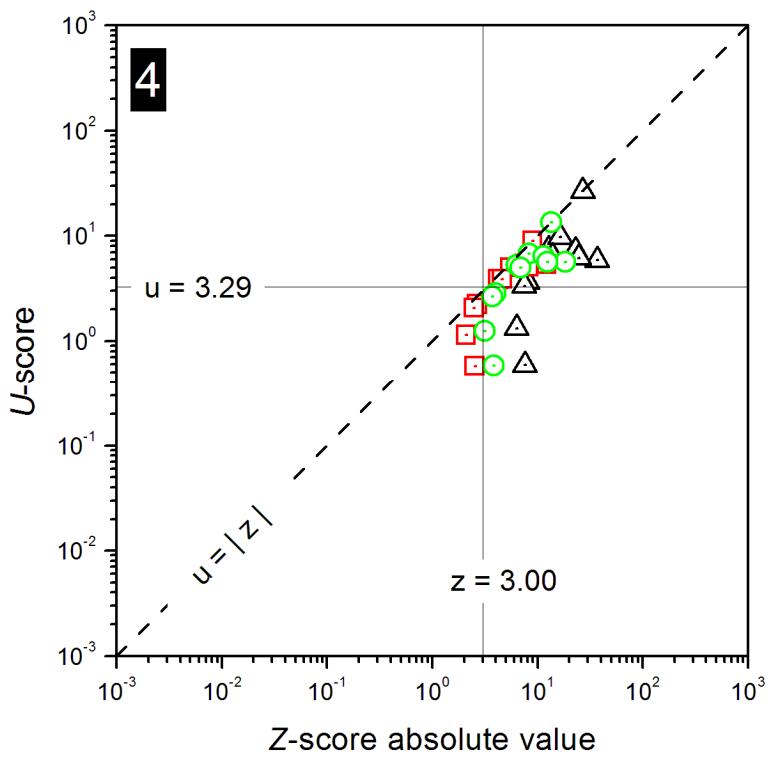


FIG. 65. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 4.

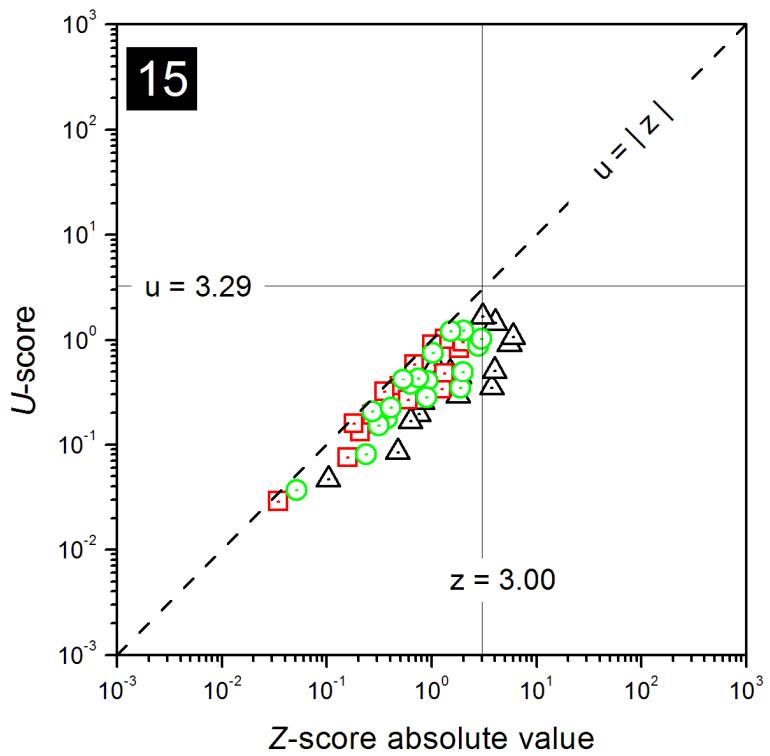


FIG. 66. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 15.

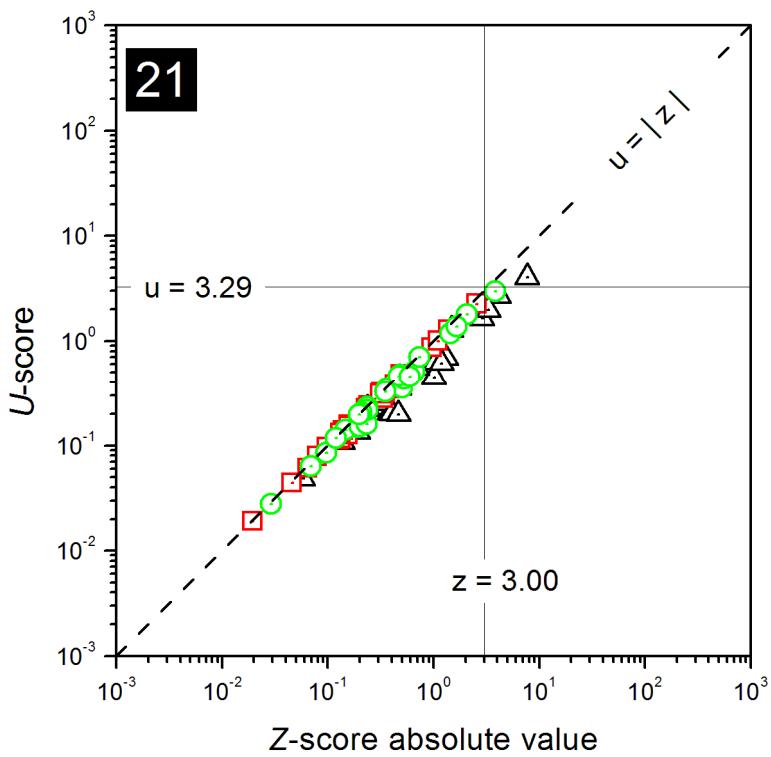


FIG. 67. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 21.

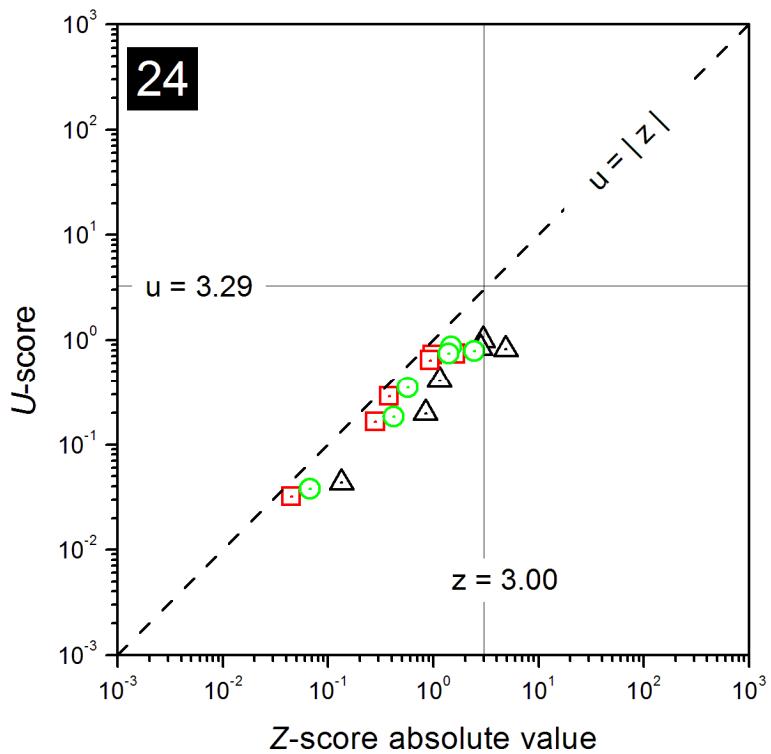


FIG. 68. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 24.

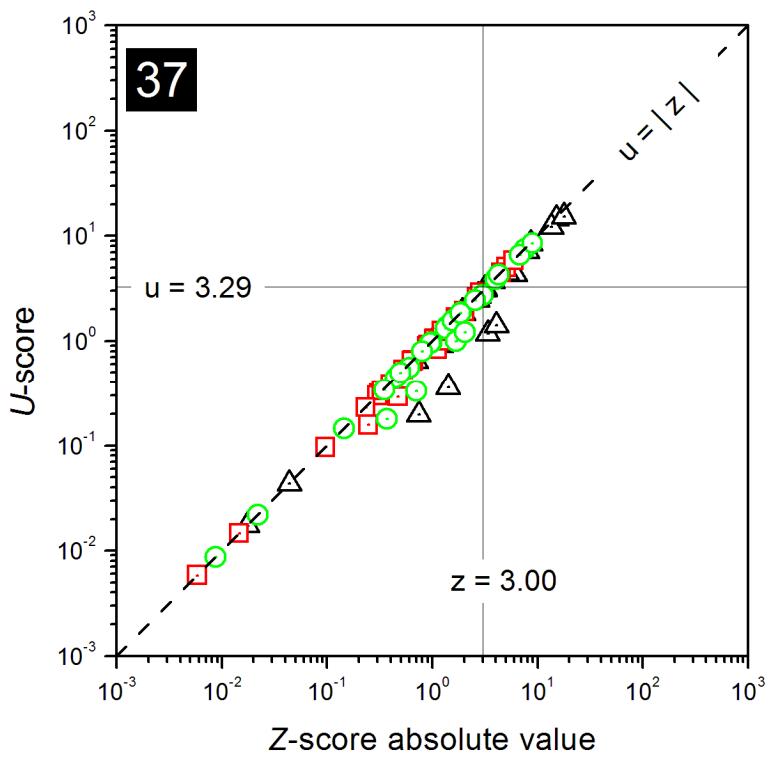


FIG. 69. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 37.

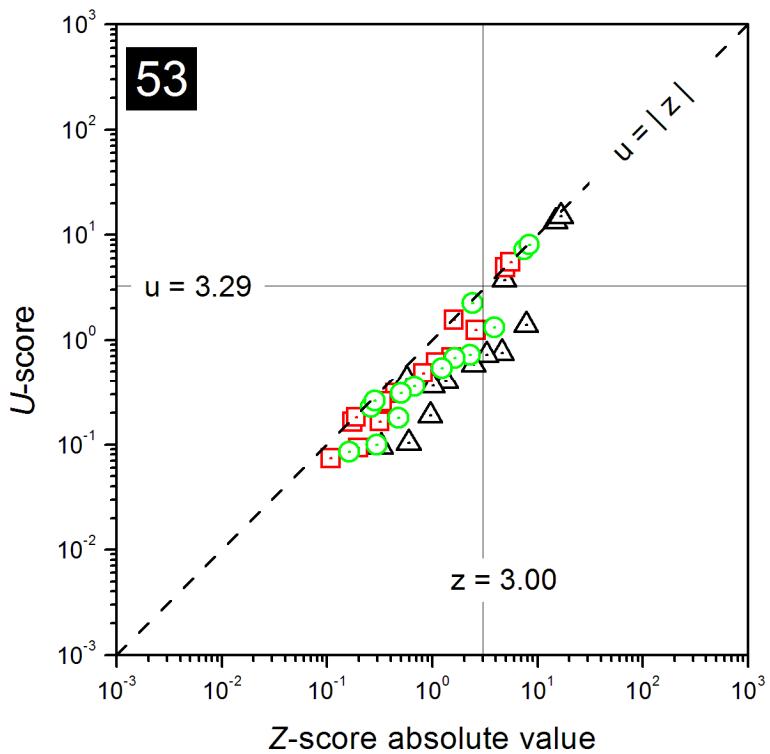


FIG. 70. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 53.

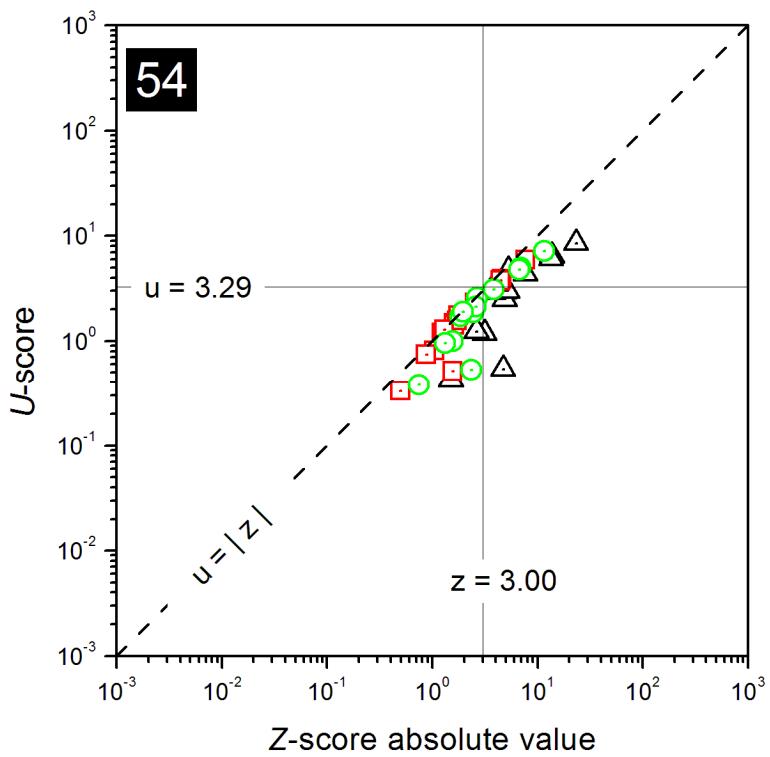


FIG. 71. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 54.

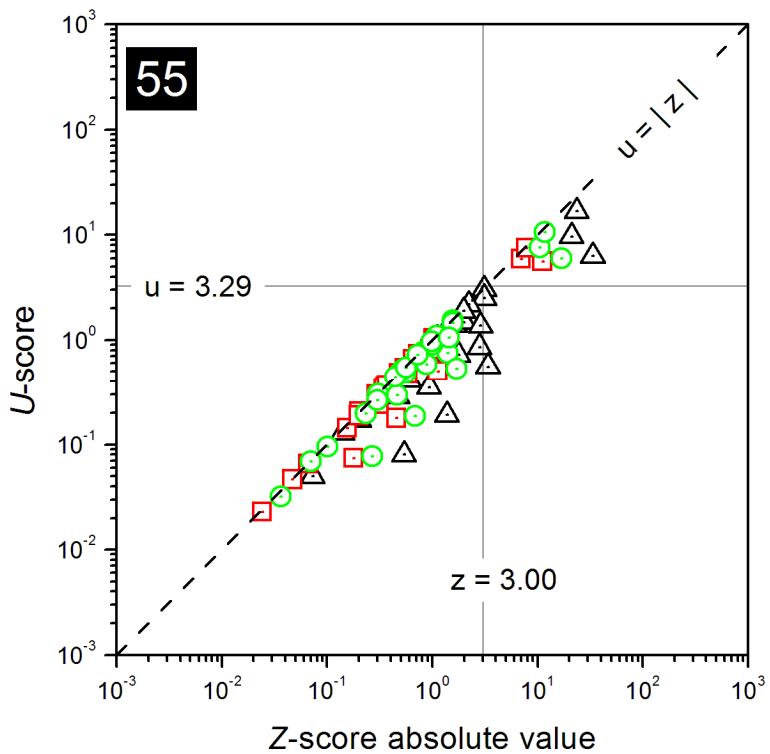


FIG. 72. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 55.

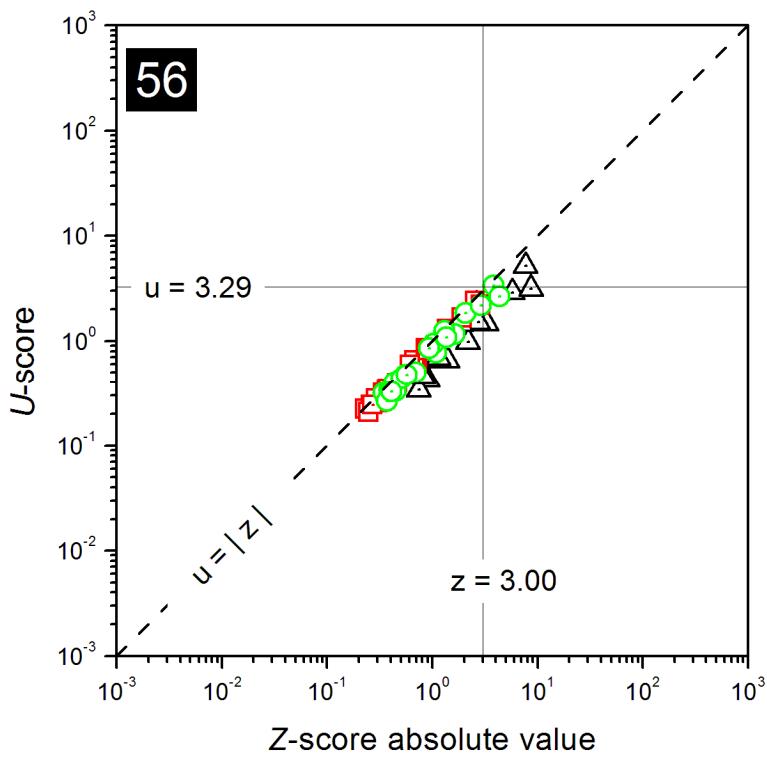


FIG. 73. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 56.

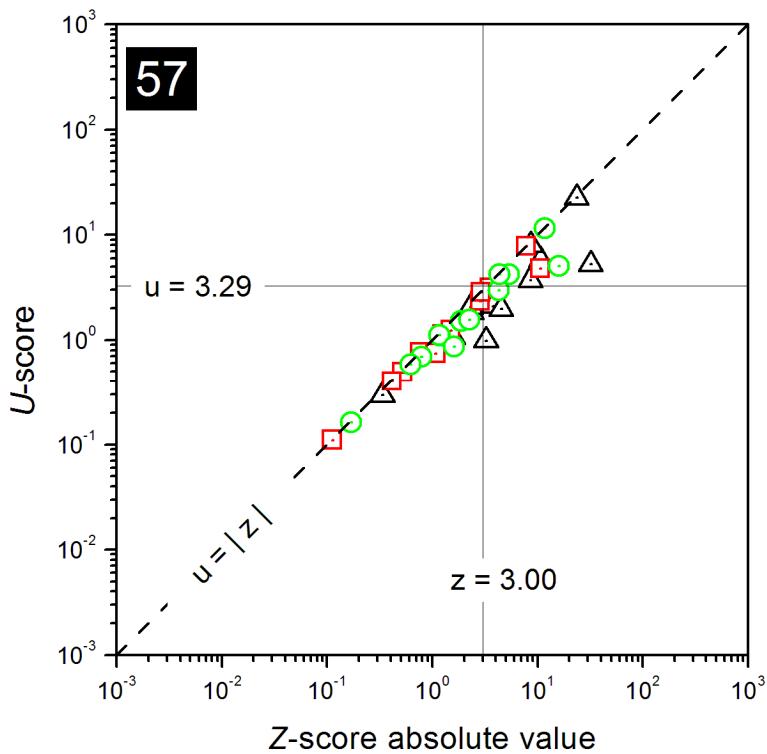


FIG. 74. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 57.

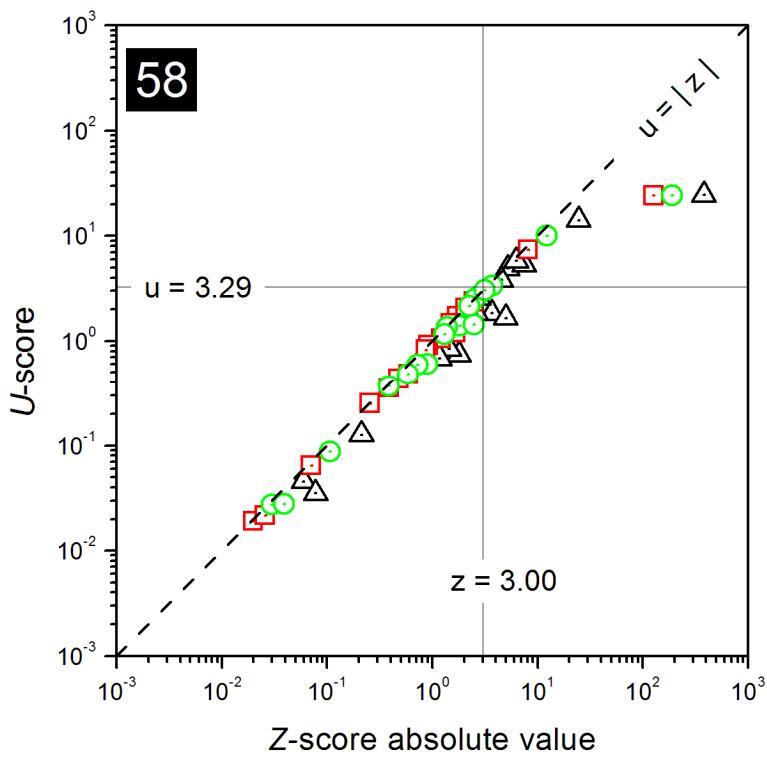


FIG. 75. Combined plots of *z*- and *u*-scores for the laboratory with code 58.

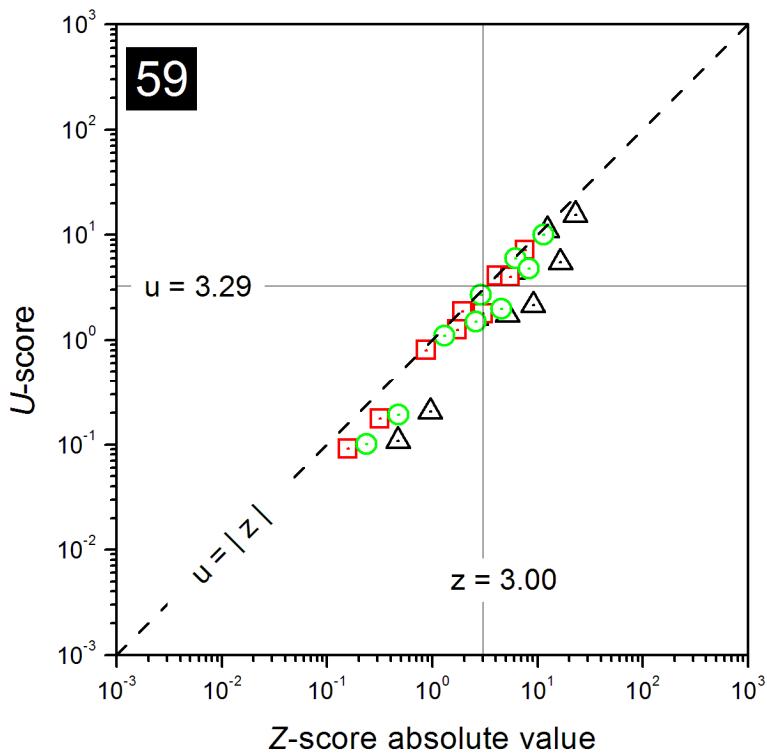


FIG. 76. Combined plots of *z*- and *u*-scores for the laboratory with code 59.

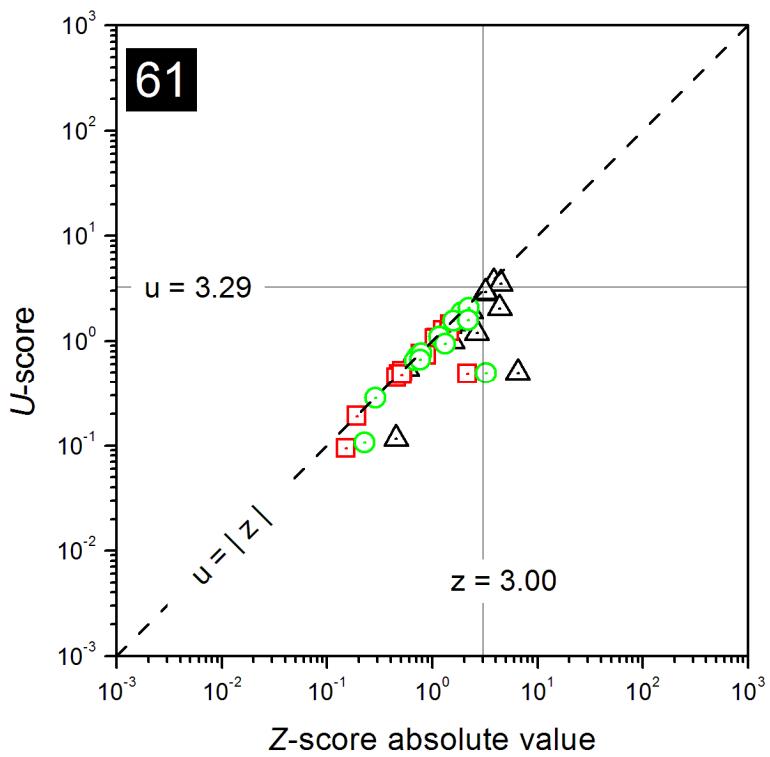


FIG. 77. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 61.

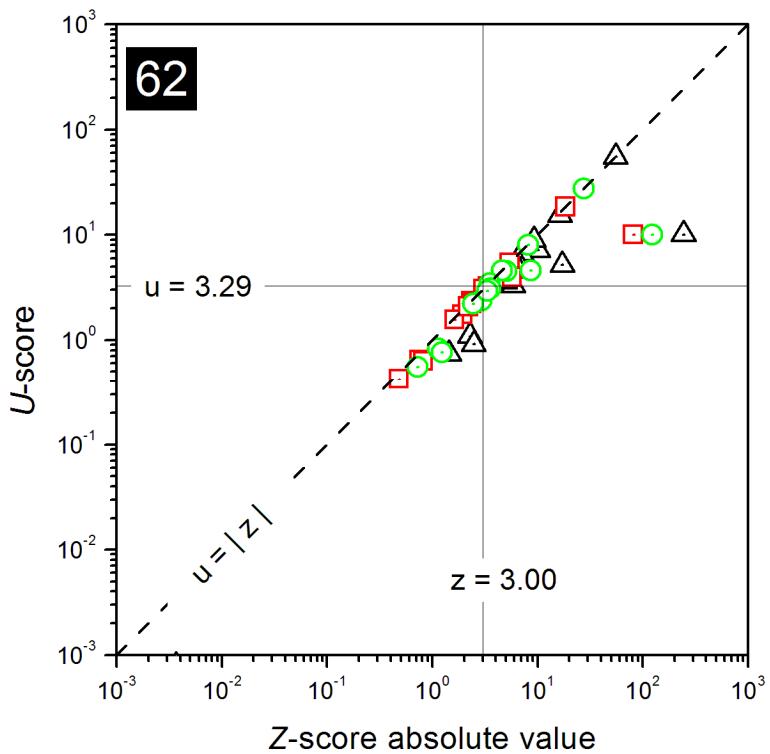


FIG. 78. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 62.

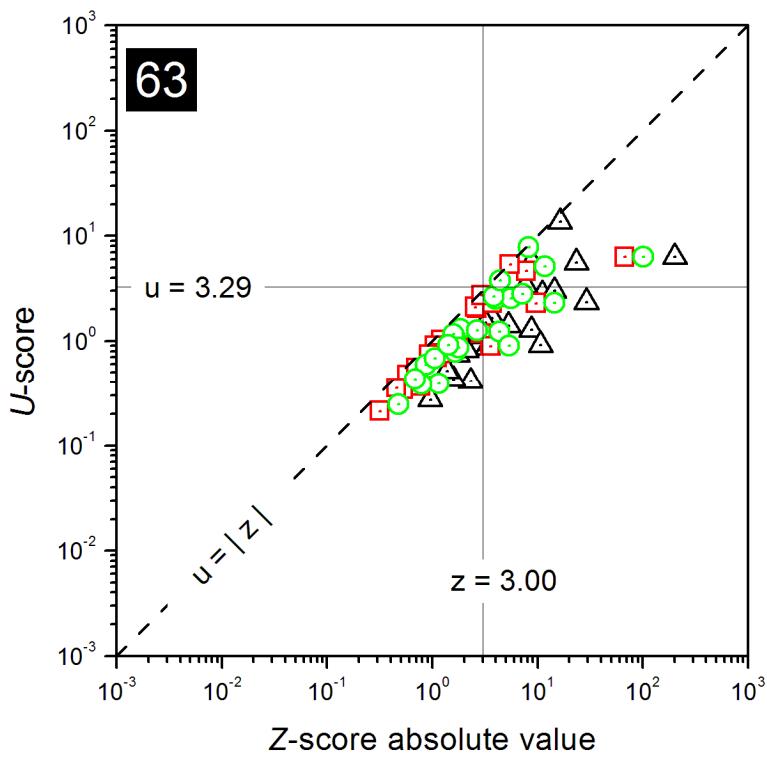


FIG. 79. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 63.

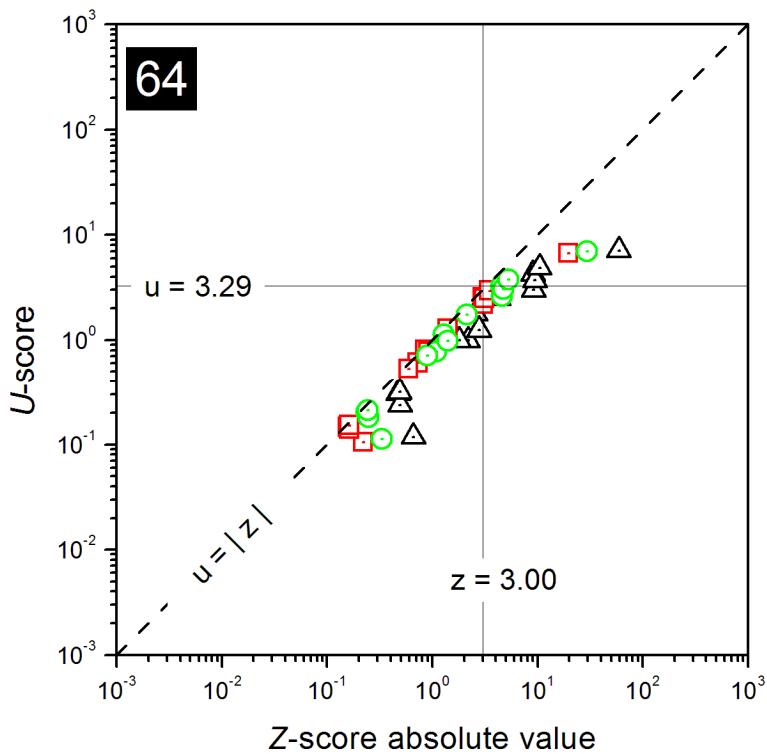


FIG. 80. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 64.

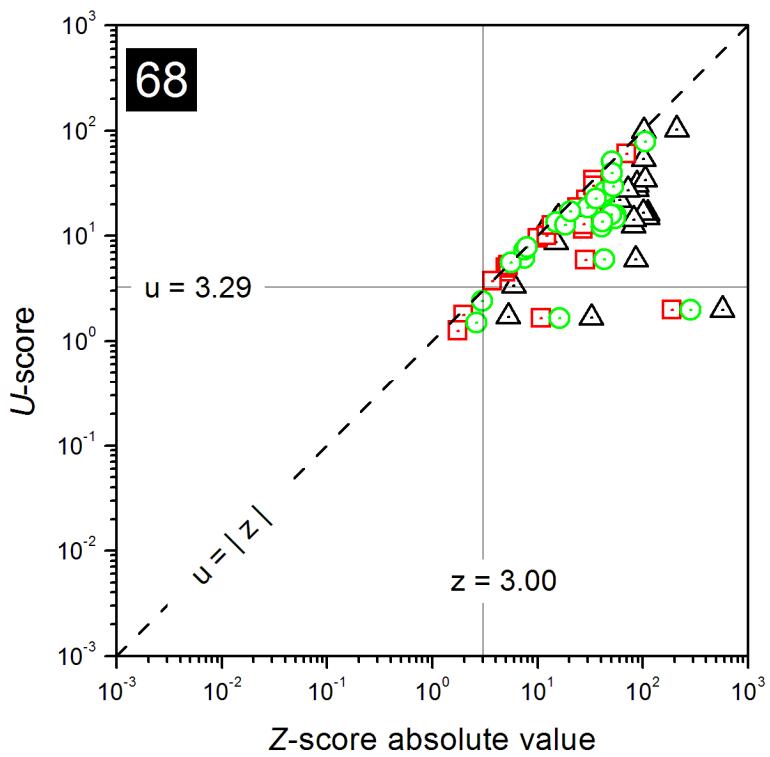


FIG. 81. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 68.

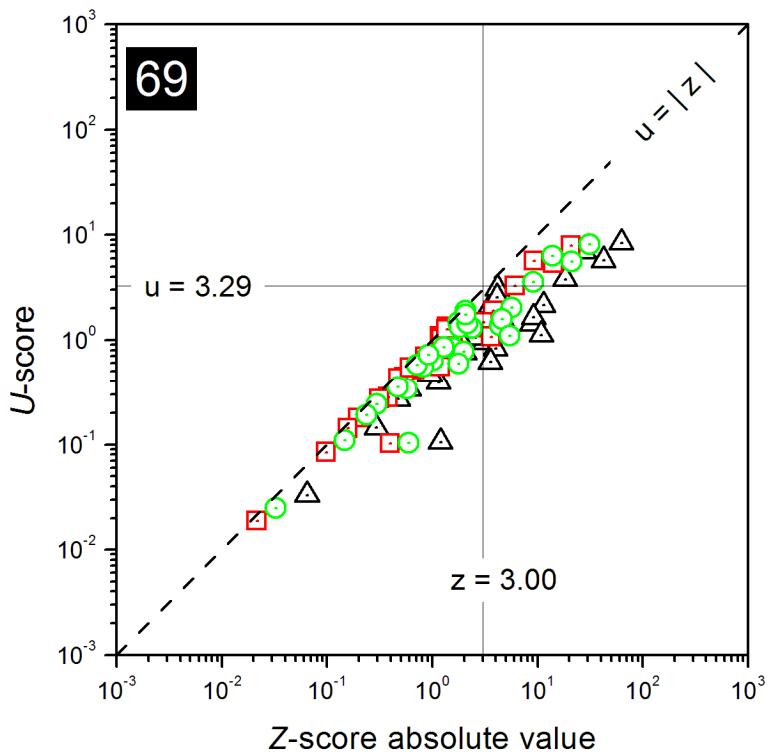


FIG. 82. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 69.

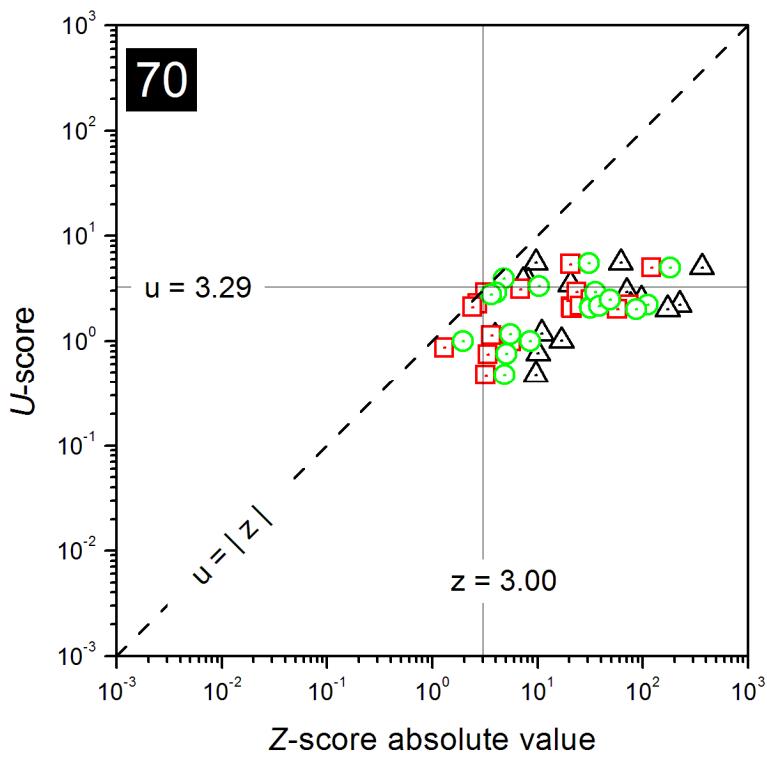


FIG. 83. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 70.

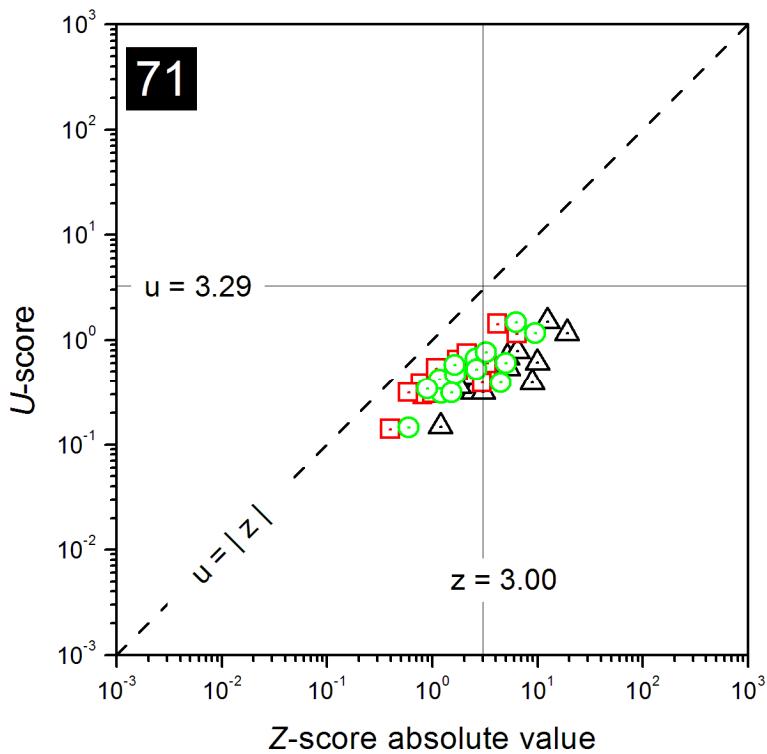


FIG. 84. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 71.

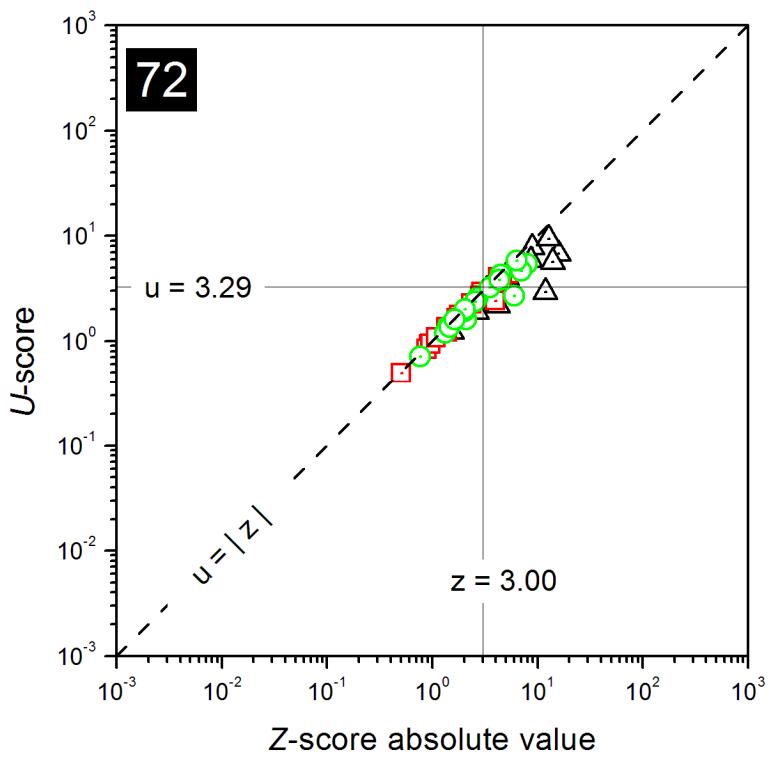


FIG. 85. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 72.

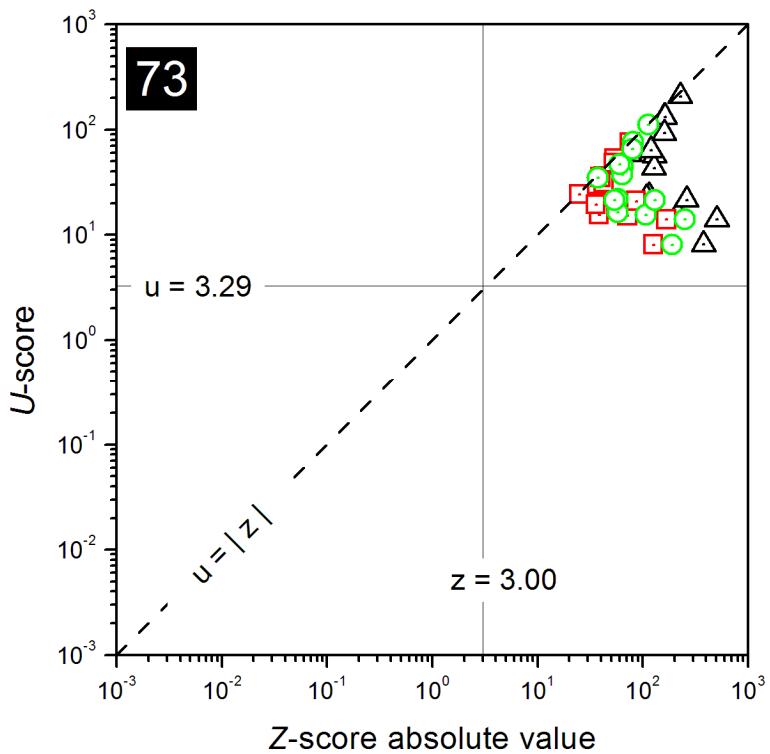


FIG. 86. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 73.

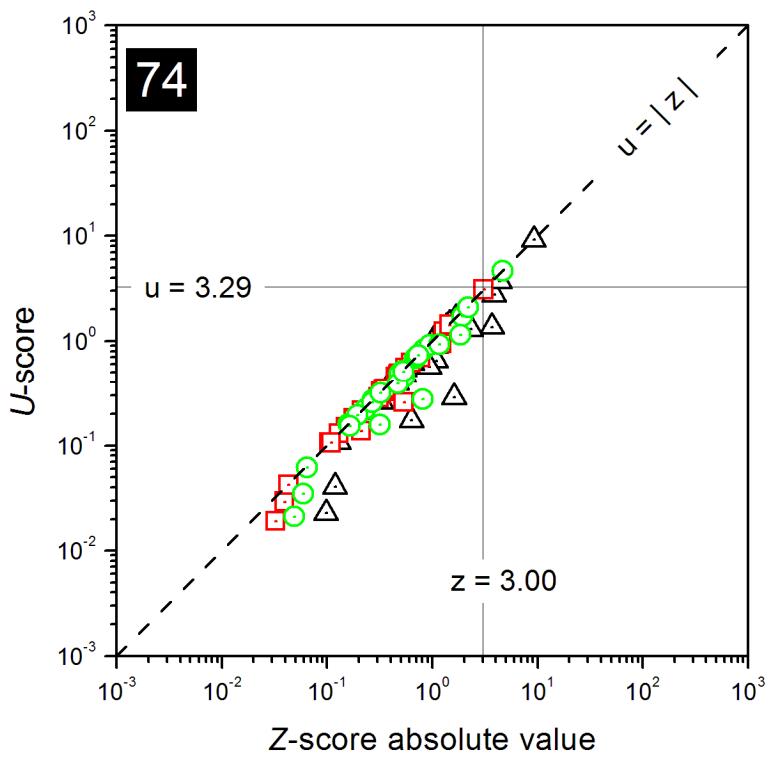


FIG. 87. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 74.

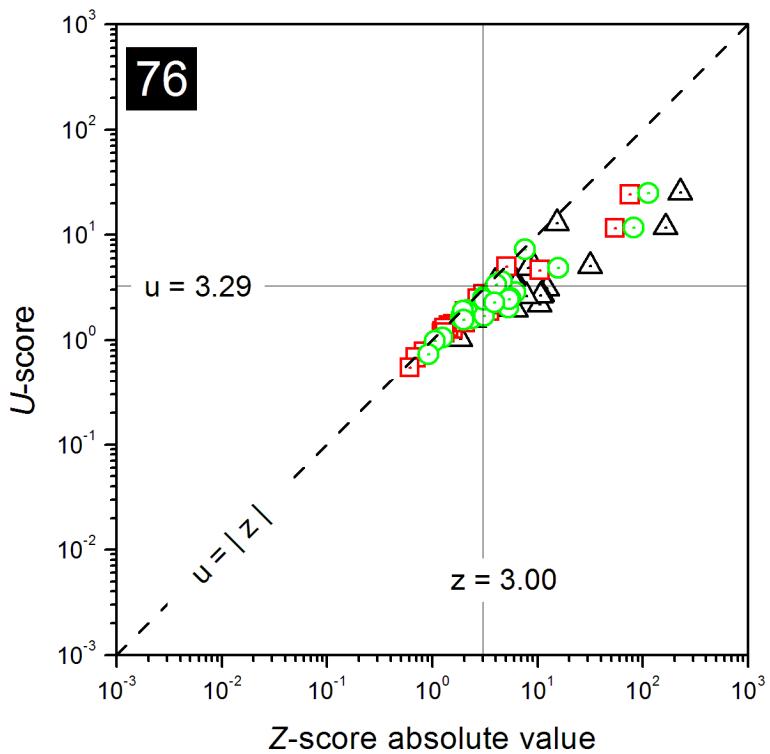


FIG. 88. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 76.

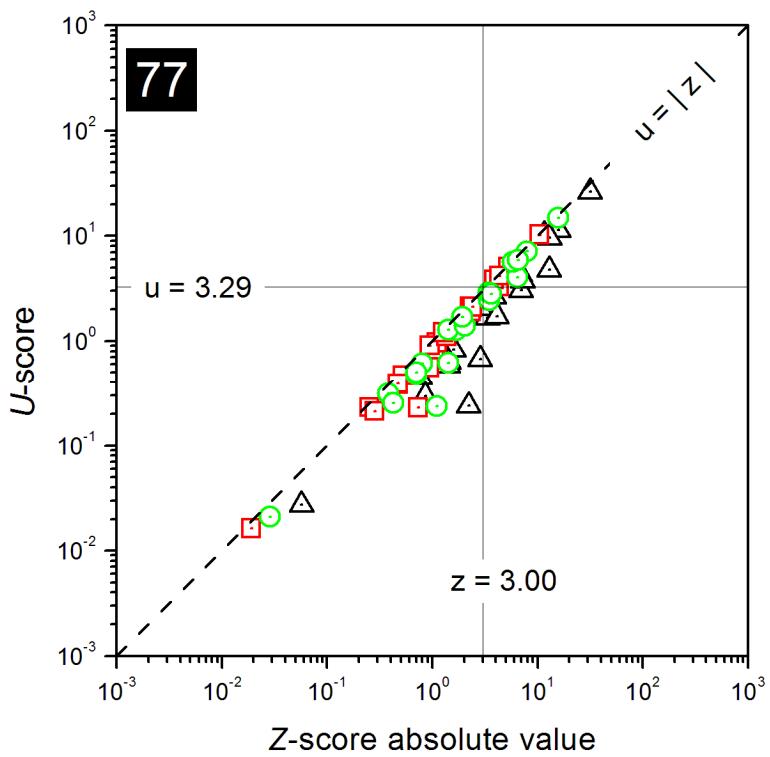


FIG. 89. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 77.

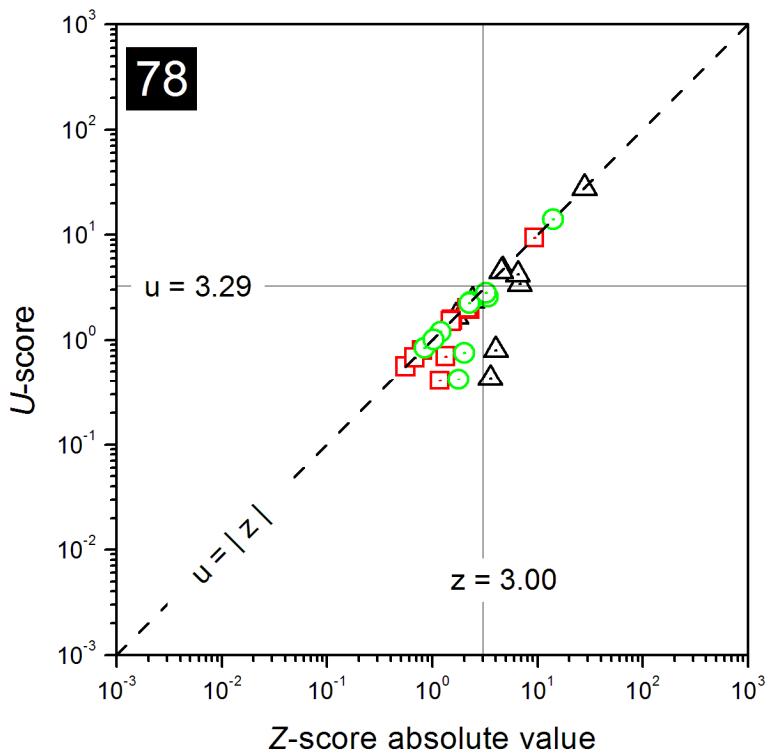


FIG. 90. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 78.

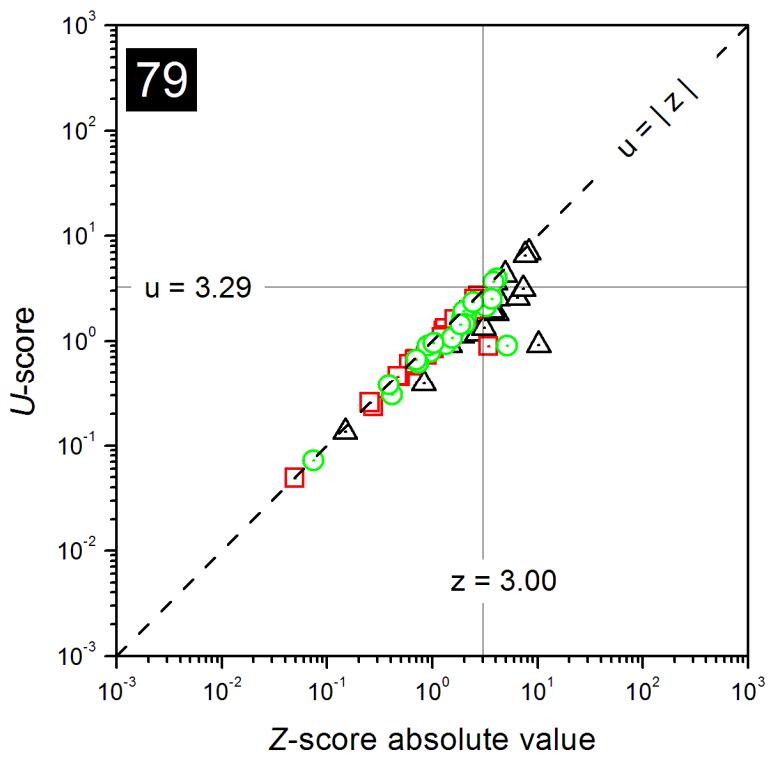


FIG. 91. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 79.

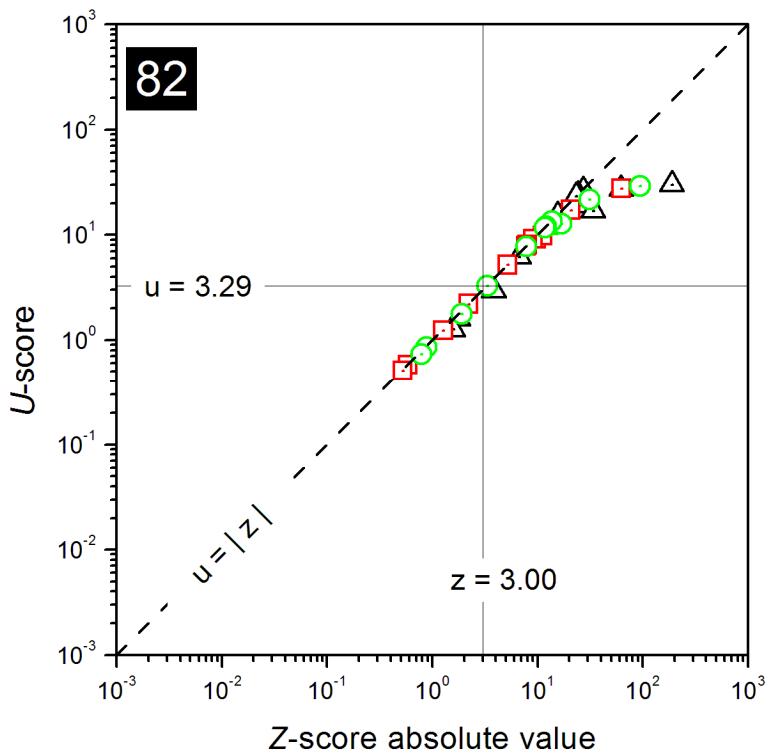


FIG. 92. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 82.

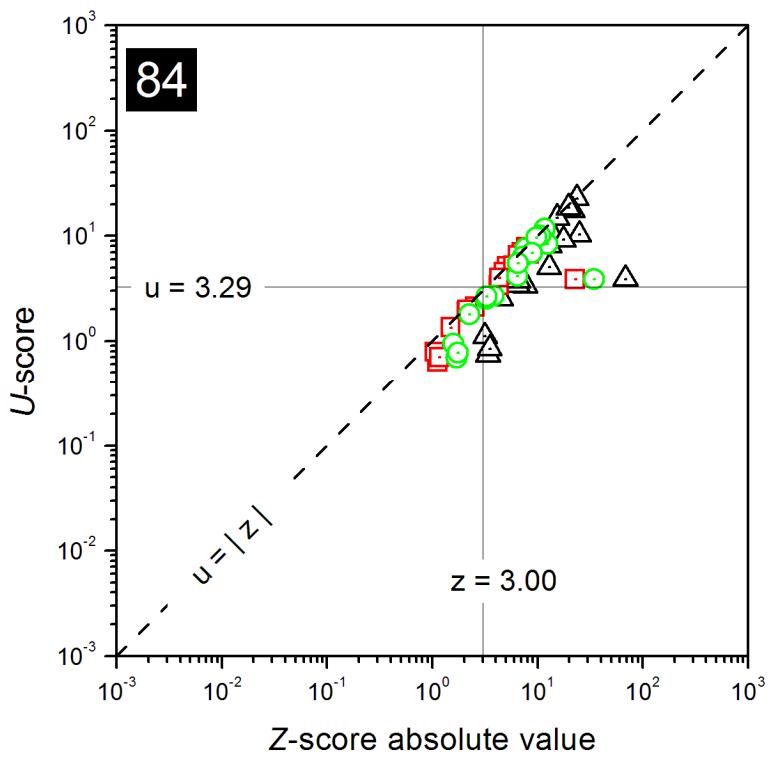


FIG. 93. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 84.

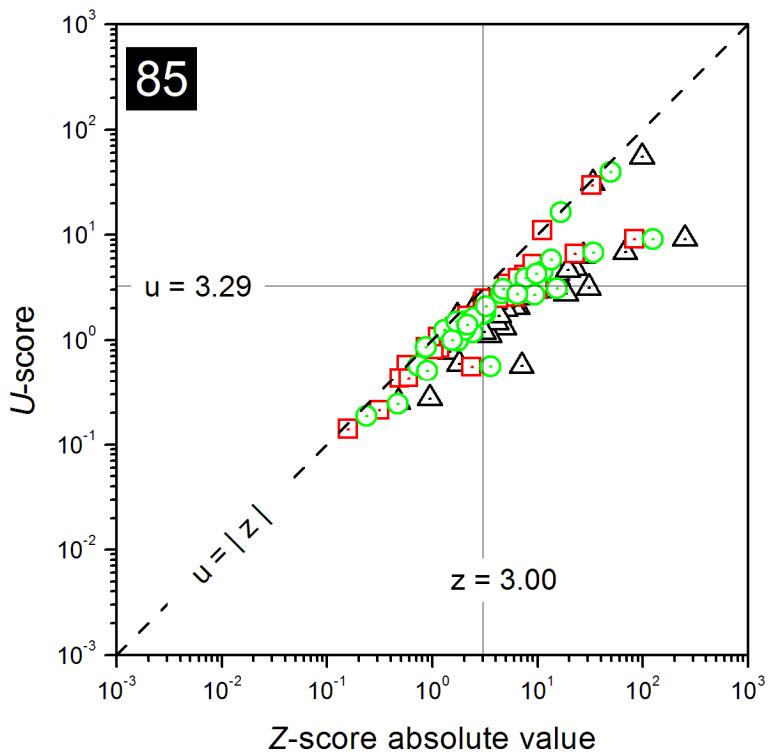


FIG. 94. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 85.

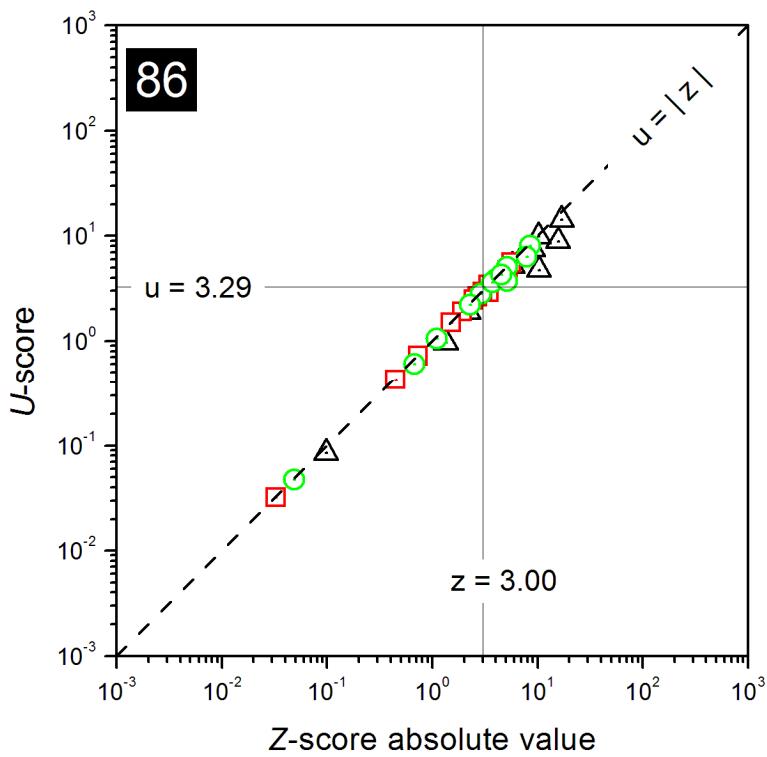


FIG. 95. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 86.

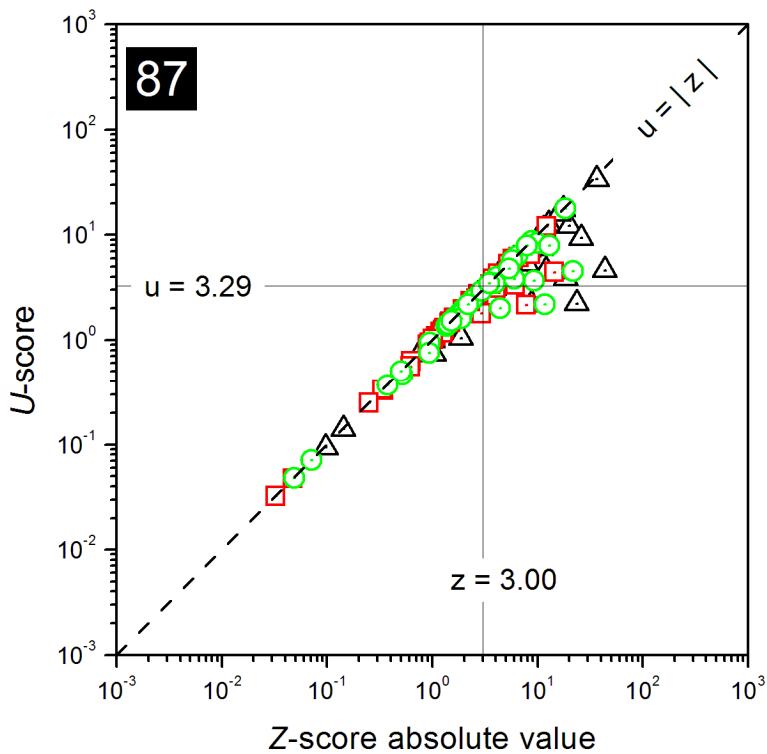
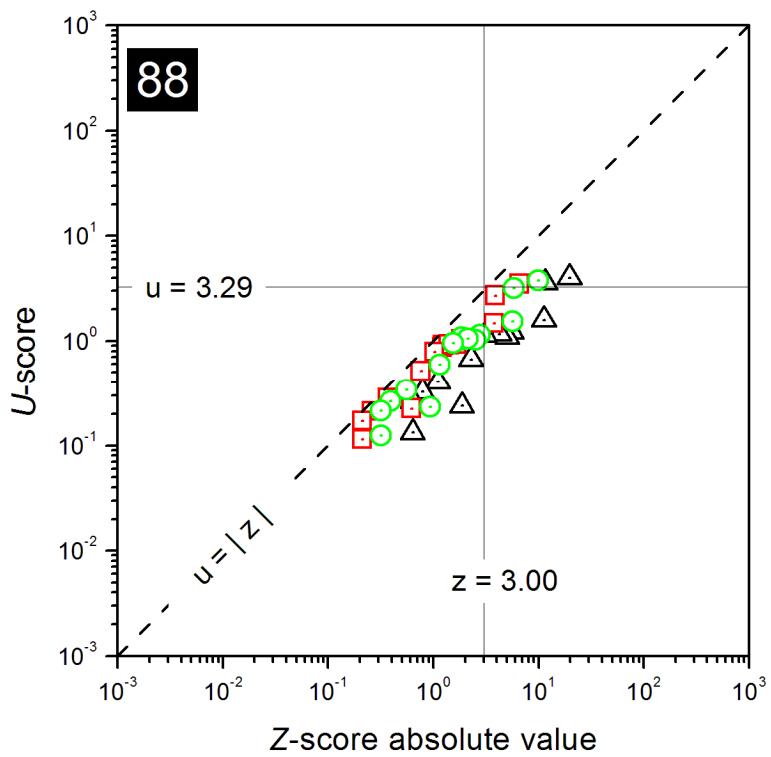
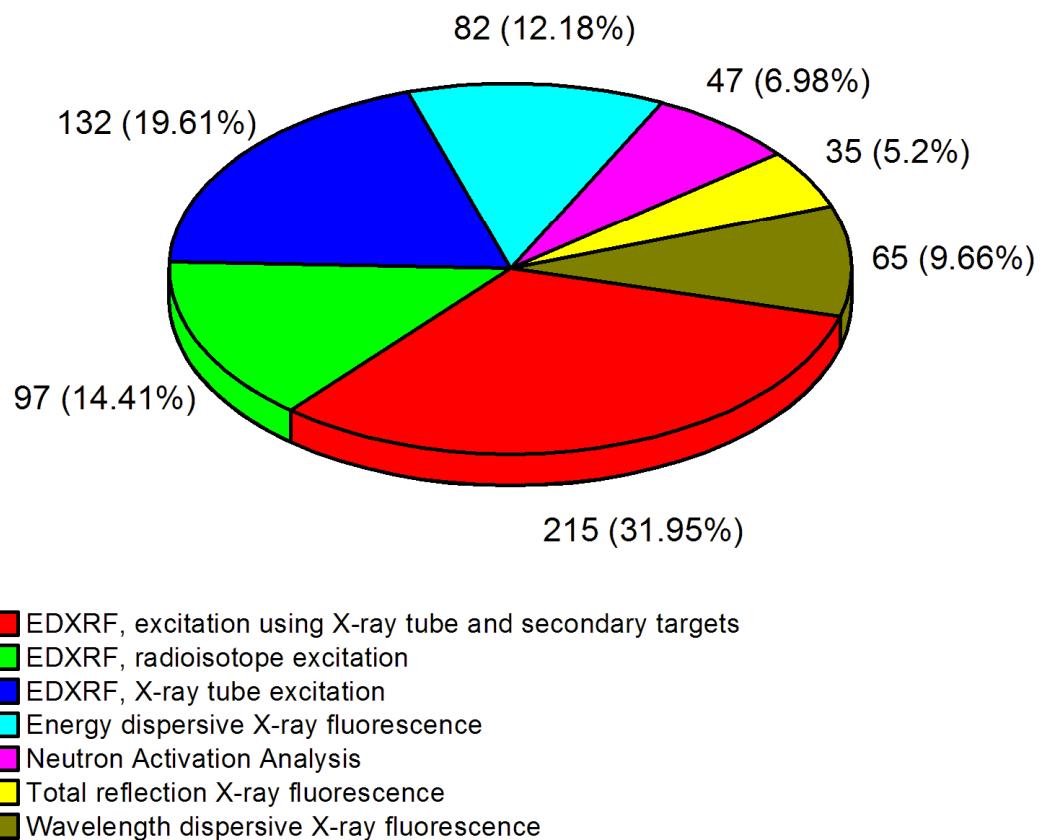


FIG. 96. Combined plots of  $z$ - and  $u$ -scores for the laboratory with code 87.



*FIG. 97. Combined plots of *z*- and *u*-scores for the laboratory with code 88.*



*FIG. 98. Utilization of analytical techniques. For each analytical technique the number of submitted results is shown. The percent values relate to the total number of 673 submitted results.*

## REFERENCES

- [1] THOMPSON, M., "Recent trends in inter-laboratory precision at ppb and sub-ppb concentrations in relation to fitness for purpose criteria in proficiency testing", *Analyst* 125 (2000) 385-386.
- [2] GRUBBS, F.E., "Procedures for detecting outlying observations in samples", *Technometrics* 11 (1969) 1-21.
- [3] INTERNATIONAL ATOMIC ENERGY AGENCY, A Nonparametric Statistical Method for the Determination of a Confidence Interval for the Mean of a Set of Results Obtained in a Laboratory Intercomparison, IAEA/RL/84, IAEA, Vienna (1981).
- [4] INTERNATIONAL ATOMIC ENERGY AGENCY, Report on the Intercomparison Run IAEA-Soil-7: Trace Elements in Soil, IAEA/RL/112, IAEA, Vienna (1984).
- [5] NATRELLA, M.G., Experimental Statistic, Handbook 91, National Bureau of Standards, United States Department of Commerce (1963).
- [6] ZIELINSKI R., Statistical Tables, PWN, Warsaw (1972).
- [7] GRUBBS, F.E., "Sample Criteria for Testing Outlying Observations", *The Annals of Mathematical Statistics* 21 (1950) 27-58.
- [8] THOMPSON, M., WOOD, R., "The international harmonized protocol for the proficiency testing of (chemical) analytical laboratories", *Journal - Association of Official Analytical Chemists*. 76 (1993) 926-940.
- [9] INTERNATIONAL ORGANIZATION FOR STANDARDIZATION, Conformity assessment –General requirements for proficiency testing, ISO/IEC/DIS 17043:2008, ISO, Geneva (2008).
- [10] HUND, E., MASSART, D.L., SMEYERS-VERBEKE, J., "Inter-laboratory studies in analytical chemistry", *Analytica Chimica Acta* 423 (2000) 145-165.



## GLOSSARY

The definitions of terms used in the proficiency testing schemes are provided. Although this terminology might be known to the participants or can be found elsewhere [8-10] the terms used in this report are clearly defined to avoid any ambiguity.

**Proficiency testing:** evaluation of participant performance against pre-established criteria by means of interlaboratory comparisons.

**True value:** the actual concentration of the analyte in the matrix.

**Assigned value:** the value of the concentration of the analyte in the matrix used as the true value by the proficiency testing coordinator in the statistical treatment of results (or the best available estimate).

**Target value for standard deviation:** a numerical value for the standard deviation of a measurement result, which has been designated as a target for measurement quality.

**Consensus value:** the mean value of the reported laboratory results after the removal of outliers.

**Standard deviation of the consensus value:** the standard deviation of the mean value of the reported laboratory results after the removal of outliers.

**Certified Reference Material:** A reference material, accompanied by a certificate, one or more of whose property values are certified by a procedure which establishes traceability to an accurate realization of the unit in which the property values are expressed, and for which each certified value is accompanied by an uncertainty at a stated level of confidence.



## **LIST OF CONTRIBUTORS TO DRAFTING AND REVIEW**

### **ORGANISERS OF THE PROFICIENCY TEST**

#### **AUSTRIA**

Migliori, A., Padilla-Alvarez, R.,  
Karydas, A.G.  
IAEA Laboratories  
Reaktor str. 1  
A-2444 Seibersdorf  
Austria

### **PARTICIPATING LABORATORIES**

#### **ALBANIA**

Civici, N.  
Institute of Nuclear Physics,  
P.O.Box 85, Qesarake,  
1001 Tirana,  
Albania

#### **ALGERIA**

Toumert, I.  
Nuclear Research Centre of Algiers (CRNA),  
2, BP 399 Alger-Gare,  
16000 Algiers,  
Algeria

#### **ARGENTINA**

Custo, G.  
Servicios Analíticos,  
Laboratorio de Fluorescencia de Rayos X,  
Comisión Nacional de Energía Atómica,  
Avenida General Paz 1499,  
1650 San Martín,  
Argentina

Jasan, R.C.  
Comisión Nacional de Energía Atómica,  
Centro Atómico Ezeiza,  
B1802AYA Ezeiza,  
Argentina

#### **BOLIVIA**

Chungara Castro, J.  
Instituto Boliviano de Ciencia  
y Tecnología Nuclear,  
Avenida 6 de Agosto 2905,  
4821 La Paz,  
Bolivia

## **BRAZIL**

Mulako Sato, I.

Instituto de Pesquisas Energéticas e Nucleares,  
Av. Prof. Lineu Prestes, 2242,  
Cidade Universitária,  
05508-000 São Paulo,  
Brazil

Parreira, P.S.

Universidade Estadual de Londrina,  
Laboratório de Física Nuclear Aplicada  
Dept. de Física/CCE,  
Caixa Postal 6001  
Campus Universitário - PR 455 Km 380  
86051-990 Londrina,  
Brazil

## **BULGARIA**

Nikolova, E.

Institut Nuclear Research Nuclear Energy,  
Tsarigradsko shosse 72,  
1784 Sofia,  
Bulgaria

## **CAMEROON**

Saïdou, S.

Nuclear Technology Section,  
Institute of Geological and Mining Research,  
P.O. Box 4110,  
Yaounde,  
Cameroon

## **CANADA**

Jovanovic, S.

Canadian Nuclear Safety Commission Lab,  
3484 Limebank Road,  
K1V 1E1 Ottawa,  
Canada

## **COSTA RICA**

Salazar, M.A.

Cicanum- Universidad De Costa Rica,  
Ciudad de la Investigación,  
Centro Investigaciones Atómicas Nucleares y  
Moleculares,  
11501-2060 San Jose,  
Costa Rica

## **CUBA**

Macías, N.M.A.

Centro de Aplicaciones Tecnológicas  
y Desarrollo Nuclear (CEADEN)  
Calle 30 # 502, esquina 5ta. Ave., Miramar,  
10400 La Habana,  
Cuba

## **GREECE**

- Rouni, P.
- Nuclear Engineering Department,  
School of Mechanical Engineering,  
National Technical University of Athens  
9 Iroon Polytechniou street, Zografos Campus,  
157 80 Zografos,  
Greece
- Ioannides, K.
- University of Ioannina,  
Department of Physics,  
45110 Ioannina,  
Greece

## **INDIA**

- Prasad, M.V.R.
- Indira Gandhi Centre for Atomic Research,  
Environment & Safety Division,  
603102 Kalpakkam,  
India
- Gupta, D.
- Saha Institute of Nuclear Physics,  
EDXRF Lab for Environmental studies,  
Nuclear Physics Division,  
1/AF Bidhannagar,  
700064 Kolkata,  
India

## **JAMAICA**

- Grant, C.
- International Centre for Environmental  
and Nuclear Sciences,  
University of the West Indies Mona Campus,  
KGN7 Kingston,  
Jamaica

## **KENIA**

- Mangala, M.J.
- University of Nairobi,  
Institute of Nuclear Science & Technology,  
P.O. BOX 30179,  
254 Nairobi,  
Kenya

## **MADAGASCAR**

- Andriambololona, R.
- Institut National des Sciences  
et Techniques Nucléaires,  
Près Bloc Technique,  
Enceinte de l'Université d'Antananarivo,  
101 Antananarivo,  
Madagascar

**MEXICO**

Zarazúa, G.

National Institute for Nuclear Research,  
Carretera México-Toluca S/N,  
52750 Ocoyoacac,  
Mexico

**MONGOLIA**

Batjargal, B.

Central Geological Laboratory,  
Songinokhairkhan district,  
Trade Union street, P.O.Box-437,  
18080 Ulaanbaatar,  
Mongolia

**PERU**

Olivera, P.

Instituto Peruano de Energia Nuclear,  
Centro Nuclear Oscar Miroquesada  
de la Guerra,  
Av. Jose Saco Km. 12,5 Carabayllo,  
Lima 6,  
Peru

**SENEGAL**

Traore, A.

Institut de Technologie Nucleaire Appliquee,  
Avenue Cheikh Anta Diop de Dakar BP.5005,  
99000 Dakar,  
Senegal

**SLOVENIA**

Kump, P.

Jozef Stefan Institute,  
Jamova 39,  
1000 Ljubljana,  
Slovenia

**SRI LANKA**

Seneviratne, M.C.S.

Atomic Energy Authority,  
No:60/460,  
Baseline Road, Orugodawatte, Wellampitiya,  
Colombo,  
Sri Lanka

**SUDAN**

Habbani, F.

Department of Physics,  
University of Khartoum,  
P.O.Box 321,  
Khartoum,  
Sudan

## **SWEDEN**

Larsson, S.

Analysis Laboratory,  
RUAG Space AB Sweden,  
Solhusgatan 11,  
SE-40515 Göteborg,  
Sweden

## **THAILAND**

Fungklin, R.

Nuclear Technology Service Center,  
Thailand Institute of Nuclear Technology,  
9/9 Moo 7 Tambol Saimul,  
26120 Ongkharak,  
Thailand

## **TURKEY**

Zararsiz, A.

Saraykoy Nuclear Research  
and Training Center,  
Saray Mah., Atom Cad., No:27, Kazan,  
6860 Ankara,  
Turkey

## **UNITED REPUBLIC OF TANZANIA**

Banzi, F.P.

Tanzania Atomic Energy Commission,  
Box 743,  
Arusha,  
United Republic of Tanzania

## **URUGUAY**

Rosario Odino, Q.F.

Laboratorio de Tecnogestión,  
Ministerio de Industria, Energía y Minería  
Hervidero 2861 entre Río Grande y Ricaurte,  
11800 Montevideo,  
Uruguay

## **VENEZUELA**

Greaves, E.D.


Universidad Simón Bolívar,  
Laboratorio de Física Nuclear,  
Valle de Sartenejas, Baruta, Edo. Miranda,  
1080 Caracas,  
Venezuela

## **VIETNAM**

Thi Kim Dung, N.

Institute for Technology of Radioactive  
and Rare Elements,  
48 Lang-Ha street,  
100000 Hanoi,  
Vietnam





## ORDERING LOCALLY

In the following countries, IAEA priced publications may be purchased from the sources listed below or from major local booksellers.

Orders for unpriced publications should be made directly to the IAEA. The contact details are given at the end of this list.

### AUSTRALIA

#### ***DA Information Services***

648 Whitehorse Road, Mitcham, VIC 3132, AUSTRALIA  
Telephone: +61 3 9210 7777 • Fax: +61 3 9210 7788  
Email: [books@dadirect.com.au](mailto:books@dadirect.com.au) • Web site: <http://www.dadirect.com.au>

### BELGIUM

#### ***Jean de Lannoy***

Avenue du Roi 202, 1190 Brussels, BELGIUM  
Telephone: +32 2 5384 308 • Fax: +32 2 5380 841  
Email: [jean.de.lannoy@euronet.be](mailto:jean.de.lannoy@euronet.be) • Web site: <http://www.jean-de-lannoy.be>

### CANADA

#### ***Renouf Publishing Co. Ltd.***

5369 Canotek Road, Ottawa, ON K1J 9J3, CANADA  
Telephone: +1 613 745 2665 • Fax: +1 643 745 7660  
Email: [order@renoufbooks.com](mailto:order@renoufbooks.com) • Web site: <http://www.renoufbooks.com>

#### ***Bernan Associates***

4501 Forbes Blvd., Suite 200, Lanham, MD 20706-4391, USA  
Telephone: +1 800 865 3457 • Fax: +1 800 865 3450  
Email: [orders@bernan.com](mailto:orders@bernan.com) • Web site: <http://www.bernan.com>

### CZECH REPUBLIC

#### ***Suweco CZ, spol. S.r.o.***

Klecakova 347, 180 21 Prague 9, CZECH REPUBLIC  
Telephone: +420 242 459 202 • Fax: +420 242 459 203  
Email: [nakup@suweco.cz](mailto:nakup@suweco.cz) • Web site: <http://www.suweco.cz>

### FINLAND

#### ***Akateeminen Kirjakauppa***

PO Box 128 (Keskuskatu 1), 00101 Helsinki, FINLAND  
Telephone: +358 9 121 41 • Fax: +358 9 121 4450  
Email: [akatilaus@akateeminen.com](mailto:akatilaus@akateeminen.com) • Web site: <http://www.akateeminen.com>

### FRANCE

#### ***Form-Edit***

5 rue Janssen, PO Box 25, 75921 Paris CEDEX, FRANCE  
Telephone: +33 1 42 01 49 49 • Fax: +33 1 42 01 90 90  
Email: [fabien.boucard@formedit.fr](mailto:fabien.boucard@formedit.fr) • Web site: <http://www.formedit.fr>

#### ***Lavoisier SAS***

14 rue de Provigny, 94236 Cachan CEDEX, FRANCE  
Telephone: +33 1 47 40 67 00 • Fax: +33 1 47 40 67 02  
Email: [livres@lavoisier.fr](mailto:livres@lavoisier.fr) • Web site: <http://www.lavoisier.fr>

#### ***L'Appel du livre***

99 rue de Charonne, 75011 Paris, FRANCE  
Telephone: +33 1 43 07 50 80 • Fax: +33 1 43 07 50 80  
Email: [livres@appeldulivre.fr](mailto:livres@appeldulivre.fr) • Web site: <http://www.appeldulivre.fr>

### GERMANY

#### ***Goethe Buchhandlung Teubig GmbH***

Schweitzer Fachinformationen  
Willstätterstrasse 15, 40549 Düsseldorf, GERMANY  
Telephone: +49 (0) 211 49 8740 • Fax: +49 (0) 211 49 87428  
Email: [s.dehaan@schweitzer-online.de](mailto:s.dehaan@schweitzer-online.de) • Web site: <http://www.goethebuch.de>

### HUNGARY

#### ***Librotade Ltd., Book Import***

PF 126, 1656 Budapest, HUNGARY  
Telephone: +36 1 257 7777 • Fax: +36 1 257 7472  
Email: [books@librotade.hu](mailto:books@librotade.hu) • Web site: <http://www.librotade.hu>

## **INDIA**

### **Allied Publishers**

1<sup>st</sup> Floor, Dubash House, 15, J.N. Heredi Marg, Ballard Estate, Mumbai 400001, INDIA  
Telephone: +91 22 2261 7926/27 • Fax: +91 22 2261 7928  
Email: alliedpl@vsnl.com • Web site: <http://www.alliedpublishers.com>

### **Bookwell**

3/79 Nirankari, Delhi 110009, INDIA  
Telephone: +91 11 2760 1283/4536  
Email: bkwell@nde.vsnl.net.in • Web site: <http://www.bookwellindia.com>

## **ITALY**

### **Libreria Scientifica "AEIOU"**

Via Vincenzo Maria Coronelli 6, 20146 Milan, ITALY  
Telephone: +39 02 48 95 45 52 • Fax: +39 02 48 95 45 48  
Email: info@libreriaaeiou.eu • Web site: <http://www.libreriaaeiou.eu>

## **JAPAN**

### **Maruzen Co., Ltd.**

1-9-18 Kaigan, Minato-ku, Tokyo 105-0022, JAPAN  
Telephone: +81 3 6367 6047 • Fax: +81 3 6367 6160  
Email: journal@maruzen.co.jp • Web site: <http://maruzen.co.jp>

## **NETHERLANDS**

### **Martinus Nijhoff International**

Koraalrood 50, Postbus 1853, 2700 CZ Zoetermeer, NETHERLANDS  
Telephone: +31 793 684 400 • Fax: +31 793 615 698  
Email: info@nijhoff.nl • Web site: <http://www.nijhoff.nl>

### **Swets Information Services Ltd.**

PO Box 26, 2300 AA Leiden  
Dellaertweg 9b, 2316 WZ Leiden, NETHERLANDS  
Telephone: +31 88 4679 387 • Fax: +31 88 4679 388  
Email: tbeyens@nl.swets.com • Web site: <http://www.swets.com>

## **SLOVENIA**

### **Cankarjeva Zalozba dd**

Kopitarjeva 2, 1515 Ljubljana, SLOVENIA  
Telephone: +386 1 432 31 44 • Fax: +386 1 230 14 35  
Email: import.books@cankarjeva-z.si • Web site: [http://www.mladinska.com/cankarjeva\\_zalozba](http://www.mladinska.com/cankarjeva_zalozba)

## **SPAIN**

### **Diaz de Santos, S.A.**

Librerias Bookshop • Departamento de pedidos  
Calle Albasanz 2, esquina Hermanos Garcia Noblejas 21, 28037 Madrid, SPAIN  
Telephone: +34 917 43 48 90 • Fax: +34 917 43 4023  
Email: compras@diazdesantos.es • Web site: <http://www.diazdesantos.es>

## **UNITED KINGDOM**

### **The Stationery Office Ltd. (TSO)**

PO Box 29, Norwich, Norfolk, NR3 1PD, UNITED KINGDOM  
Telephone: +44 870 600 5552  
Email (orders): books.orders@tso.co.uk • (enquiries): book.enquiries@tso.co.uk • Web site: <http://www.tso.co.uk>

## **UNITED STATES OF AMERICA**

### **Bernan Associates**

4501 Forbes Blvd., Suite 200, Lanham, MD 20706-4391, USA  
Telephone: +1 800 865 3457 • Fax: +1 800 865 3450  
Email: orders@bernan.com • Web site: <http://www.bernan.com>

### **Renouf Publishing Co. Ltd.**

812 Proctor Avenue, Ogdensburg, NY 13669, USA  
Telephone: +1 888 551 7470 • Fax: +1 888 551 7471  
Email: orders@renoufbooks.com • Web site: <http://www.renoufbooks.com>

### **United Nations**

300 East 42<sup>nd</sup> Street, IN-919J, New York, NY 1001, USA  
Telephone: +1 212 963 8302 • Fax: 1 212 963 3489  
Email: publications@un.org • Web site: <http://www.unp.un.org>

## **Orders for both priced and unpriced publications may be addressed directly to:**

IAEA Publishing Section, Marketing and Sales Unit, International Atomic Energy Agency  
Vienna International Centre, PO Box 100, 1400 Vienna, Austria  
Telephone: +43 1 2600 22529 or 22488 • Fax: +43 1 2600 29302  
Email: sales.publications@iaea.org • Web site: <http://www.iaea.org/books>





INTERNATIONAL ATOMIC ENERGY AGENCY  
VIENNA  
ISSN 2074-7659